

March 2004

# RNeasy<sup>®</sup> 96 Universal Tissue Handbook

For high-throughput RNA purification from all types of  
animal tissue



WWW.QIAGEN.COM

Trademarks: QIAGEN®, QIAamp®, BioRobot®, HotStarTaq®, MagAttract®, MinElute™, Omniscript®, QuantiProbe™, QuantiTect®, RNAprotect™, RNeasy®, Sensiscript® (QIAGEN Group); ABI PRISM® (Applied Biosystems); Electrapette®, Impact®, Matrix® (Matrix Technologies Corp.); LightCycler® (Roche Group); PAXgene™ (PreAnalytiX GmbH); SYBR® (Molecular Probes); Yakima Yellow™ (Epoch Biosciences).

BioRobot workstations and QIAGEN kits are intended as general-purpose devices. No claim or representation is intended for their use in identifying any specific organism or for a specific clinical use (diagnostic, prognostic, therapeutic, or blood banking). It is the user's responsibility to validate the performance of BioRobot workstations and QIAGEN kits for any particular use, since their performance characteristics have not been validated for any specific organism. BioRobot workstations and QIAGEN kits may be used in clinical diagnostic laboratory systems after the laboratory has validated their complete system as required by CLIA '88 regulations in the U.S. or equivalents in other countries. QIAGEN Robotic Systems are not available in all countries; please inquire.

Purchase of QIAGEN products for PCR containing Taq DNA Polymerase or HotStarTaq DNA Polymerase is accompanied by a limited license to use them in the Polymerase Chain Reaction (PCR) process for research and development activities in conjunction with a thermal cycler whose use in the automated performance of the PCR process is covered by the up-front license fee, either by payment to Applied Biosystems or as purchased, i.e. an authorized thermal cycler. The PCR process is covered by U.S. Patents 4,683,195 and 4,683,202 and foreign equivalents owned by Hoffmann-La Roche AG. The 5' nuclease process is covered by patents owned by Roche Molecular Systems, Inc. and F. Hoffmann-La Roche Ltd. The purchase of QIAGEN's DNA oligos conveys no license, either expressly or by implication, to the purchaser or subsequent user to use the PCR process.

Molecular Beacons are licensed under patents owned by The Public Health Research Institute of the City of New York, Inc. and come with licensed rights for use only in the purchaser's research and development activities.

QIAzol Lysis Reagent is a subject of US Patent No. 5,346,994 and foreign equivalents.

Differential display technology is covered by US patent No. 5,262,311 and other pending patents licensed to GenHunter Corporation.

© 2004 QIAGEN, all rights reserved.

# Contents

|   |           |
|---|-----------|
| <b>Kit Contents</b>   | <b>4</b>  |
| <b>Storage</b>  | <b>4</b>  |
| <b>Product Use Limitations</b>  | <b>5</b>  |
| <b>Product Warranty and Satisfaction Guarantee</b>                                  | <b>5</b>  |
| <b>Technical Assistance</b>   | <b>5</b>  |
| <b>Safety Information</b>   | <b>6</b>  |
| <b>Quality Control</b>  | <b>6</b>  |
| <b>Introduction</b>   | <b>7</b>  |
| Principle and procedure   | 7         |
| Description of protocols  | 9         |
| <b>Equipment and Reagents to Be Supplied by User</b>                                | <b>10</b> |
| Tissuelyser system  | 11        |
| Centrifuge 4K15C  | 11        |
| QIAvac 96 vacuum manifold   | 12        |
| <b>Important Notes</b>  | <b>15</b> |
| Amount of tissue  | 15        |
| Handling and storage of starting material   | 16        |
| Disruption and homogenization of starting materials                                 | 17        |
| Square-well blocks  | 18        |
| <b>Protocols</b>  |           |
| ■ <b>Purification of Total RNA from Animal Tissues Using Vacuum/Spin Technology</b> | <b>19</b> |
| ■ <b>Purification of Total RNA from Animal Tissues Using Spin Technology</b>        | <b>24</b> |
| <b>Troubleshooting Guide</b>  | <b>29</b> |
| <b>Appendix A: General Remarks on Handling RNA</b>                                  | <b>33</b> |
| <b>Appendix B: Storage, Quantification, and Determination of Quality of RNA</b>     | <b>35</b> |
| <b>Appendix C: Protocol for Formaldehyde Agarose Gel Electrophoresis</b>            | <b>38</b> |
| <b>Appendix D: Optional On-Plate DNase Digestion with the RNase-Free DNase Set</b>  | <b>40</b> |
| <b>References</b>   | <b>42</b> |
| <b>Ordering Information</b>   | <b>43</b> |
| <b>QIAGEN Distributors</b>  | <b>55</b> |

## Kit Contents

| <b>RNeasy 96 Universal Tissue Kit</b> | <b>(4)</b>    | <b>(12)</b>    |
|---------------------------------------|---------------|----------------|
| <b>Catalog no.</b>                    | <b>74881</b>  | <b>74882</b>   |
| <b>Number of preps</b>                | <b>4 x 96</b> | <b>12 x 96</b> |
| RNeasy 96 Plates                      | 4             | 12             |
| Register Cards (96-well)              | 4             | 12             |
| Collection Microtubes (racked)        | 4 x 96        | 12 x 96        |
| Collection Microtube Caps             | 100 x 8       | 320 x 8        |
| Square-Well Blocks (2.2 ml)           | 6             | 14             |
| Elution Microtubes CL                 | 4 x 96        | 12 x 96        |
| Caps for Strips                       | 50 x 8        | 165 x 8        |
| AirPore Tape Sheets                   | 3 x 5         | 2 x 25         |
| Buffer RW1 *                          | 2 x 220 ml    | 4 x 400 ml     |
| Buffer RPE†                           | 4 x 55 ml     | 8 x 65 ml      |
| RNase-Free Water                      | 2 x 50 ml     | 12 x 30 ml     |
| QIAzol Lysis Reagent**†               | 2 x 200 ml    | 5 x 200 ml     |
| Handbook                              | 1             | 1              |

\* Not compatible with disinfecting reagents containing bleach. Contains a guanidine salt. See page 6 for safety information.

† Buffer RPE is supplied as a concentrate. Add 4 volumes of ethanol (96–100%) before use to obtain a working solution.

‡ Packaged separately.

Additional QIAzol Lysis Reagent, square-well blocks, elution microtubes, collection microtubes (racked), and AirPore Tape Sheets are available separately. See ordering information (pages 44–45).

## Storage

The RNeasy 96 Universal Tissue Kit should be stored dry at room temperature (15–25°C) and is stable for at least 9 months under these conditions.

QIAzol Lysis Reagent can be stored at room temperature or at 2–8°C and is stable for at least 12 months under these conditions.

## Product Use Limitations

RNeasy 96 Universal Tissue Kits are intended as general-purpose devices. No claim or representation is intended for their use to identify any specific organism or for clinical use (diagnostic, prognostic, therapeutic, or blood banking). It is the user's responsibility to validate the performance of RNeasy 96 Universal Tissue Kits for any particular use, since the performance characteristics of these kits have not been validated for any specific organism. RNeasy 96 Universal Tissue Kits may be used in clinical diagnostic laboratory systems after the laboratory has validated their complete system as required by CLIA '88 regulations in the U.S. or equivalents in other countries.

All due care and attention should be exercised in the handling of the products. We recommend all users of QIAGEN® products to adhere to the NIH guidelines that have been developed for recombinant DNA experiments, or to other applicable guidelines.

## Product Warranty and Satisfaction Guarantee

QIAGEN guarantees the performance of all products in the manner described in our product literature. The purchaser must determine the suitability of the product for its particular use. Should any product fail to perform satisfactorily due to any reason other than misuse, QIAGEN will replace it free of charge or refund the purchase price. We reserve the right to change, alter, or modify any product to enhance its performance and design. If a QIAGEN product does not meet your expectations, simply call your local Technical Service Department or distributor. We will credit your account or exchange the product — as you wish.

A copy of QIAGEN terms and conditions can be obtained on request, and is also provided on the back of our invoices. If you have questions about product specifications or performance, please call QIAGEN Technical Services or your local distributor (see back cover).

## Technical Assistance

At QIAGEN we pride ourselves on the quality and availability of our technical support. Our Technical Service Departments are staffed by experienced scientists with extensive practical and theoretical expertise in molecular biology and the use of QIAGEN products. If you have any questions or experience any difficulties regarding RNeasy 96 Universal Tissue Kits or QIAGEN products in general, please do not hesitate to contact us.

QIAGEN customers are a major source of information regarding advanced or specialized uses of our products. This information is helpful to other scientists as well as to the researchers at QIAGEN. We therefore encourage you to contact us if you have any suggestions about product performance or new applications and techniques.

For technical assistance and more information please call one of the QIAGEN Technical Service Departments or local distributors (see back cover).

## Safety Information

When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, please consult the appropriate material safety data sheets (MSDSs). These are available online in convenient and compact PDF format at [www.qiagen.com/ts/msds.asp](http://www.qiagen.com/ts/msds.asp) where you can find, view, and print the MSDS for each QIAGEN kit and kit component.

**CAUTION: DO NOT add bleach or acidic solutions directly to the sample-preparation waste.**

QIAzol Lysis Reagent contains guanidine thiocyanate and Buffer RW1 contains between 2.5 and 10% guanidine thiocyanate, which can form highly reactive compounds when combined with bleach.

If liquid containing these reagents is spilt, clean with suitable laboratory detergent and water. If the spilt liquid contains potentially infectious agents, clean the affected area first with laboratory detergent and water, and then with 1% (v/v) sodium hypochlorite. The following risk and safety phrases apply to the components of the RNeasy 96 Universal Tissue Kit.

### QIAzol Lysis Reagent

Contains phenol, guanidine thiocyanate: toxic, corrosive. Risk and safety phrases: \* R20-24/25-32-34, S13-26-36/37/39-45

### Buffer RW1

Contains ethanol: flammable. Risk phrase: \* R10

### 24-hour emergency information

Emergency medical information in English, French, and German can be obtained 24 hours a day from:

Poison Information Center Mainz, Germany

Tel: +49-6131-19240

## Quality Control

As part of the stringent QIAGEN quality assurance program, the performance of RNeasy 96 Universal Tissue Kits is monitored routinely on a lot-to-lot basis. All components are tested separately to ensure highest performance and reliability.

\* R10: Flammable; R20: Harmful by inhalation; R24/25: Toxic in contact with skin and if swallowed; R32: Contact with acids liberates very toxic gas; R34: Causes burns; S13: Keep away from food, drink and animal feeding stuffs; S26: In case of contact with eyes, rinse immediately with plenty of water and seek medical advice; S36/37/39: Wear suitable protective clothing, gloves and eye/face protection; S45: In case of accident or if you feel unwell, seek medical advice immediately (show the label where possible).

## Introduction

The RNeasy 96 Universal Tissue Kit is well-suited for simultaneous purification of 96 or 192 RNA samples from all types of animal or human tissue. The RNeasy 96 Universal Tissue Kit facilitates efficient, high-throughput RNA sample preparation for research use (see “Product Use Limitations”, page 5).

In less than 2 hours (including homogenization and RNA purification), 96 high-purity RNA samples can be obtained. The RNeasy 96 Universal Tissue procedure replaces current time-consuming and tedious methods involving alcohol-precipitation steps or large numbers of washing steps. The purified RNA is ready to use in any downstream application including:

- RT-PCR
- Quantitative RT-PCR, including QIAGEN QuantiTect® technology
- Differential display
- cDNA synthesis
- Northern, dot, and slot blot analysis
- Primer extension
- Poly A<sup>+</sup> RNA selection
- RNase/S1 nuclease protection
- Microarrays


## Principle and procedure

The RNeasy 96 Universal Tissue Kit represents an advanced technology for high-throughput RNA preparation. This technology integrates efficient phenol/guanidine-based lysis and silica-gel-membrane purification with the speed of vacuum and/or spin processing.

Tissue is first efficiently lysed using QIAzol Lysis Reagent and the TissueLyser. This provides rapid and parallel disruption of cells and inactivation of RNases to ensure purification of intact RNA. After phase separation by centrifugation and recovery of the aqueous phase, ethanol is added to provide appropriate binding conditions. The sample is then applied to the wells of the RNeasy 96 Universal Tissue plate, where total RNA binds and contaminants are efficiently washed away. High-performance RNA is then eluted in a small volume of water, ready for use in any downstream application.

With the RNeasy 96 Universal Tissue procedure (Figure 1), all RNA molecules longer than 200 nucleotides are purified. The procedure provides an enrichment for mRNA since most RNAs <200 nucleotides (such as 5.8S rRNA, 5S rRNA, and tRNAs, which together comprise 15–20% of total RNA) are selectively excluded. The size distribution of purified RNA is comparable to that obtained by centrifugation through a CsCl cushion, where small RNAs do not sediment efficiently.

## RNeasy 96 Universal Tissue Procedure

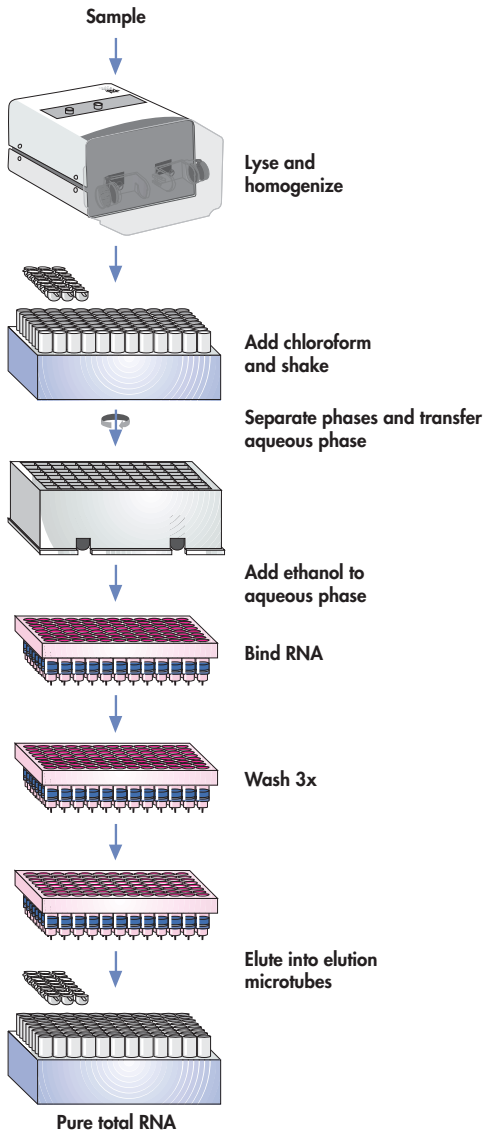

**Figure 1** RNA purification with the RNeasy 96 Universal Tissue Kit. Protocol steps can be performed in a specially designed centrifuge system (pages 11–12) with optional use of the QIAvac 96 vacuum manifold (pages 12–14).



## Description of protocols

The protocols in this handbook provide 2 different handling options, using a combination of vacuum and spin technology or spin technology alone. Both handling options provide high yields of high-performance RNA.

### I. Vacuum/spin technology

Using vacuum/spin technology, all protocol steps from the binding step to the first Buffer RPE wash step are performed on the QIAvac 96 vacuum manifold (see pages 12–14). Phase separation, the final Buffer RPE wash step, including membrane drying, and the elution steps are performed in the Centrifuge 4K15C (see pages 11–12). The Plate Rotor 2 x 96 holds 2 RNeasy 96 plates, allowing up to 192 RNA samples to be prepared in parallel. Residual traces of salt are removed by centrifugation in the final wash step. RNA purified using vacuum/spin technology can be used for any non-enzymatic or enzymatic downstream application, including quantitative RT-PCR analysis by QuantiTect technology.\*

### II. Spin technology

Using spin technology, all protocol steps are performed in the Centrifuge 4K15C (see pages 11–12). The Plate Rotor 2 x 96 holds 2 RNeasy 96 plates, allowing up to 192 RNA samples to be prepared in parallel. RNA purified using spin technology can be used for any non-enzymatic or enzymatic downstream application, including quantitative RT-PCR analysis by QuantiTect technology.\*

\* For more information about quantitative, real-time RT-PCR, request our application guide *Critical Factors for Successful Real-Time RT-PCR*.

## Equipment and Reagents to Be Supplied by User

When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

### For all protocols

- Multichannel pipet with tip. For the most efficient sample processing in the RNeasy 96 Universal Tissue protocol, we recommend the use of an electric multichannel pipet with a minimum capacity of 650  $\mu$ l per pipet tip. Good options are the Matrix® Impact® or the Matrix Multi-8 Electrapette® cordless electronic multichannel pipets, both of which have a unique expandable tip-spacing system allowing the user to transfer liquid directly from racks of tubes to 96-well microplates. Matrix Impact or Multi-8 Electrapette pipets can be purchased from Matrix Technologies Corporation ( [www.matrixtechcorp.com](http://www.matrixtechcorp.com) ).\*
- Reagent reservoirs for multichannel pipets (**Note:** Make sure that reagent reservoirs used for chloroform are chloroform-resistant.)
- Disposable gloves
- QIAGEN TissueLyser system, comprising the TissueLyser, the TissueLyser Adapter Set 2 x 96, Stainless Steel Beads, 5 mm, and the TissueLyser 5 mm Bead Dispenser, 96-Well (see page 11). Alternatively, a rotor–stator homogenizer can be used.
- Centrifuge 4K15C (see pages 11–12)
- Plate Rotor 2 x 96 (see pages 11–12)
- Chloroform (without added isoamyl alcohol)
- 96–100% ethanol<sup>†</sup>
- 70% ethanol in water<sup>†</sup>
- Dry ice
- **Optional:** Additional square-well blocks (cat. no. 19573). Two square-well blocks are supplied with the kit for use as waste-trays. If several RNeasy 96 plates are processed per day, it may be convenient to keep extra square-well blocks on hand.

### For protocol using vacuum/spin technology

- QIAvac 96 vacuum manifold (see pages 12–14)
- Vacuum source capable of generating a vacuum pressure of –800 to –900 mbar (see pages 12–14). Vacuum pumps (18 liter/min) can be purchased from KNF Neuberger ( [www.knf.com](http://www.knf.com) ).\*

\* This is not a complete list of suppliers and does not include many important vendors of biological supplies.

<sup>†</sup> Do not use denatured alcohol, which contains other substances such as methanol or methylethylketone.

## Optional reagents

- RNase-Free DNase Set (cat. no. 79254), containing RNase-free DNase I, Buffer RDD, and RNase-free water. For optional on-plate DNase digestion, the RNeasy 96 Universal Tissue procedure requires 2 RNase-Free DNase Sets per 96-well plate.

## TissueLyser system

The TissueLyser system provides high-throughput processing for simultaneous, rapid, and effective disruption of up to 192 biological samples, including all types of animal tissue. Processing of up to 2 x 96 samples takes as little as 2–5 minutes.

Disruption and homogenization using the TissueLyser gives yields comparable or better than with traditional rotor–stator homogenization methods. With rotor–stator homogenization, the samples must be processed individually, and the rotor–stator homogenizer must be cleaned after each sample to prevent cross-contamination. In contrast, the TissueLyser provides simultaneous disruption for high-throughput processing of a variety of animal tissues.

The TissueLyser system includes a number of different accessories for ease of use with different sample sizes and throughputs. In the RNeasy 96 Universal Tissue procedure, the TissueLyser Adapter Set 2 x 96 allows simultaneous processing of up to 192 samples in collection microtubes. Stainless steel beads with a diameter of 5 mm are optimal to use for animal tissues in combination with the RNeasy 96 Universal Tissue Kit. The TissueLyser 5 mm Bead Dispenser, 96-Well, is also available to conveniently deliver 96 beads in parallel into collection microtubes. See page 43 for ordering information.

## Centrifuge 4K15C


RNeasy 96 Universal Tissue protocols utilize a streamlined centrifugation procedure that allows preparation of RNA from up to 2 x 96 samples in parallel for direct use in any downstream application. For optimal handling, QIAGEN, in cooperation with the centrifuge manufacturer Sigma Laborzentrifugen GmbH, has developed a centrifugation system consisting of the Plate Rotor 2 x 96, and the refrigerated table-top Centrifuge 4K15C (see ordering information, page 43). A temperature of 4°C is necessary during phase separation for optimal removal of genomic DNA. A wide range of other rotors can be used with Centrifuge 4K15C in addition to the Plate Rotor 2 x 96.

Standard table-top centrifuges and 96-well–microplate rotors are not suitable for the RNeasy 96 Universal Tissue procedure. Usually 96-well–microplate buckets are not deep enough to carry the complete RNeasy assembly without interfering with how the buckets swing out. Furthermore, high *g*-forces (>5500 x *g*) are required for optimal performance of the RNeasy 96 Universal Tissue procedure.

For further information about the centrifuge and rotor please contact QIAGEN or your local distributor.

**Warning:** Do not centrifuge the Plate Rotor 2 x 96 metal holders without the RNeasy 96 plates and square-well blocks, collection microtubes, or elution microtubes. If unsupported, the holders will collapse under high  $g$ -force. Therefore, remove the holders during test runs. Standard 96-well microplates may be centrifuged in the holders if a  $g$ -force of  $500 \times g$  is not exceeded.

## QIAvac 96 vacuum manifold

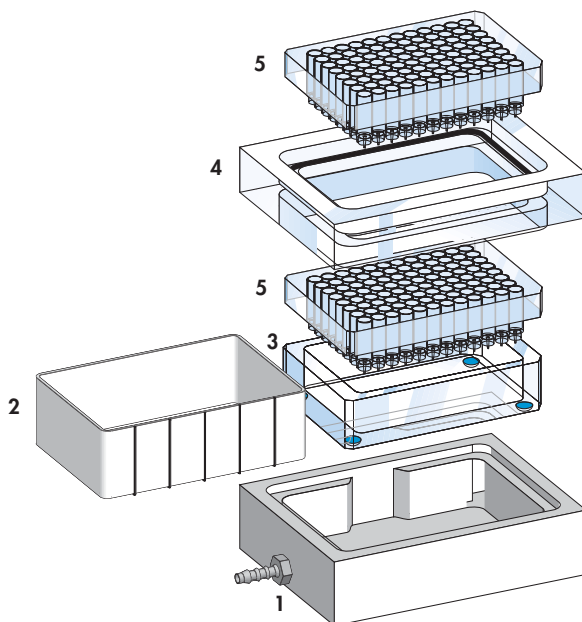

**Figure 2** Components of the QIAvac 96 vacuum manifold.

1. QIAvac base, which holds a waste tray, a plate holder, or a microtube rack
2. Waste tray
3. Plate holder (shown with 96-well plate) — not used in RNeasy 96 Universal Tissue protocols
4. QIAvac 96 top plate with aperture for 96-well plate
5. 96-well plate\*

\* Not included with QIAvac 96. Included in the RNeasy 96 Universal Tissue Kit.

## QIAvac 96 handling guidelines

QIAvac 96 facilitates the RNeasy 96 Universal Tissue procedure by providing a convenient, modular vacuum manifold (Figure 2) for use with the RNeasy 96 Universal Tissue Kit. The following recommendations should be followed when handling the QIAvac 96 vacuum manifold.

- QIAvac 96 operates with a house vacuum or a vacuum pump. If the house vacuum is weak or inconsistent, we recommend using a vacuum pump with a capacity of 18 liter/min. Use of insufficient vacuum pressure may reduce RNA yield and purity.
- A vacuum pressure of  $-800$  to  $-900$  mbar should develop when an RNeasy 96 plate sealed with tape is used on the QIAvac 96. Vacuum pressures exceeding  $-900$  mbar should be avoided. The vacuum pressure is the pressure differential between the inside of the manifold and the atmosphere (standard atmospheric pressure: 1013 millibar or 760 mm Hg) and can be regulated and measured using a pressure gauge or vacuum regulator (see ordering information, page 44). Vacuum recommendations are given in negative units to indicate the required reduction in pressure with respect to the atmosphere. Table 1 provides pressure conversions to other units.
- Between loading steps, the vacuum must be switched off and the manifold ventilated to maintain uniform conditions for each sample. This can be done with a vacuum regulator (see ordering information, page 44) inserted between the vacuum source and the QIAvac 96 vacuum manifold.
- Wear safety glasses when working near a manifold under pressure.
- For safety reasons, do not use 96-well plates that have been damaged in any way.
- Always place the QIAvac 96 vacuum manifold on a secure bench top or work area. If dropped, the manifold may crack.
- Always store the QIAvac 96 vacuum manifold clean and dry. To clean, simply rinse all components with water, and dry with paper towels. Do not air dry, as the screws may rust and need to be replaced. Do not use abrasives. After rinsing and drying, wipe manifold components with paper towels wetted with 70% ethanol, and dry with fresh paper towels.
- The QIAvac 96 vacuum manifold and components are not resistant to ethanol, methanol, or other organic solvents when exposed for long periods. If solvents are spilled on the unit, rinse thoroughly with distilled water after the RNeasy preparation. Ensure that no residual buffers remain in the vacuum manifold.
- To ensure consistent performance, do not apply silicone or vacuum grease to any part of the QIAvac 96 vacuum manifold. The spring lock on the top plate and the self-sealing gasket provide an airtight seal when vacuum is applied to the assembled unit. To maximize gasket life, rinse the gasket free of salts and buffers after each use, and dry with paper towels before storage.

**Table 1. Pressure Conversions**

| <b>To convert from millibars (mbar) to:</b> | <b>Multiply by:</b> |
|---|---------------------|
| Millimeters of mercury (mm Hg)              | 0.75                |
| Kilopascals (kPa)                           | 0.1                 |
| Inches of mercury (inch Hg)                 | 0.0295              |
| Torrs (Torr)                                | 0.75                |
| Atmospheres (atmos)                         | 0.000987            |
| Pounds per square inch (psi)                | 0.0145              |

# Important Notes

## Amount of tissue

Using the correct amount of starting material is essential in order to obtain high yields of pure RNA with the RNeasy 96 Universal Tissue Kit. The maximum amount that can be used is limited by:

- the volume of QIAzol Lysis Reagent required for efficient lysis and the maximum loading volume of the RNeasy 96 Universal Tissue plate
- the RNA binding capacity of the RNeasy 96 Universal Tissue plate wells (100 µg)
- the type of tissue

The RNeasy 96 Universal Tissue procedure is optimized for use with a maximum of 50 mg animal tissue (flash-frozen). With adipose tissue, up to 100 mg can be used. With liver, thymus, spleen, or RNA<sub>later</sub><sup>™</sup> stabilized tissues,\* only 25 mg should be used in order to avoid clogging the RNeasy 96 Universal Tissue plate.

Table 2 gives specifications for the RNeasy 96 Universal Tissue plate. Each well of the plate has a maximum binding capacity of 100 µg of RNA, but actual yields depend on the sample type used. Table 3 gives examples of expected RNA yields from various tissues.

**Table 2. RNeasy 96 Universal Tissue Plate Specifications**

|                                 |   |
|---------------------------------|---|
| Preps per plate                 | 96  |
| Amount of starting material     | 50 mg (up to 100 mg adipose tissue; 25 mg flash-frozen liver, thymus, or spleen tissue; 25 mg RNA <sub>later</sub> stabilized tissue) |
| Binding capacity per well       | 100 µg RNA <sup>†</sup>   |
| Maximum loading volume per well | 1 ml  |
| RNA size distribution           | All RNA >200 nucleotides  |

<sup>†</sup> Yields are limited by tissue type and amount. The maximum binding capacity of 100 µg RNA is usually not reached (see text).

**Note:** If the binding capacity of the RNeasy 96 Universal Tissue plate is exceeded, yields of total RNA will not be consistent and less than 100 µg total RNA may be recovered. If lysis of the starting material is incomplete, yields of total RNA will be lower than expected, even if the binding capacity of the RNeasy 96 Universal Tissue plate is not exceeded.

\* See the RNA<sub>later</sub> Handbook for more information about RNA<sub>later</sub> RNA Stabilization Reagent.

Weighing tissue is the most accurate way to quantify the amount of starting material. However, the following may be used as a guide.

A 3 mm cube (approximately this size: ; volume, 27 mm<sup>3</sup>) of most animal tissues weighs 25–35 mg.

**Table 3. Typical Total RNA Yields Using the RNeasy 96 Universal Tissue Kit**

| Tissue         | RNA yield (µg per 10 mg of tissue)* |
|----------------|-------------------------------------|
| Kidney         | 5–40                                |
| Liver          | 15–80                               |
| Lung           | 5–15                                |
| Heart          | 5–25                                |
| Muscle         | 5–35                                |
| Brain          | 5–20                                |
| Adipose tissue | 0.5–2.5                             |
| Spleen         | 15–100                              |
| Intestine      | 10–60                               |
| Skin           | 2–5                                 |

\* Amounts can vary due to species, age, gender, physiological state, etc. Since the RNeasy procedure enriches for RNA >200 bases long, the total RNA yield does not include 5.8S rRNA, tRNA, and other low-molecular weight RNAs, which make up 15–20% of total cellular RNA.

## Handling and storage of starting material

RNA is not protected until the sample material is treated with RNA*later* RNA Stabilization Reagent, flash-frozen, or disrupted and homogenized in the presence of RNase-inhibiting or denaturing agents. It is therefore important that samples are immediately frozen in liquid nitrogen<sup>†</sup> and stored at –70°C or immediately immersed in RNA*later* RNA Stabilization Reagent.

Frozen tissue should not be allowed to thaw during handling or weighing. The relevant procedures should be carried out as quickly as possible.

<sup>†</sup> When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.



## Disruption and homogenization of starting materials

Efficient disruption and homogenization of the starting material is an absolute requirement for all total RNA purification procedures. Disruption and homogenization are 2 distinct steps.

**Disruption:** Complete disruption of plasma membranes of cells and organelles is absolutely required to release all the RNA contained in the sample. Different samples require different methods to achieve complete disruption. Incomplete disruption results in significantly reduced yields.

**Homogenization:** Homogenization is necessary to reduce the viscosity of the lysates produced by disruption. Homogenization shears high-molecular-weight genomic DNA and other high-molecular-weight cellular components to create a homogeneous lysate. Incomplete homogenization results in inefficient binding of RNA to the RNeasy membrane and therefore significantly reduced yields.

Some disruption methods simultaneously homogenize the sample while others require an additional homogenization step. Table 4 gives an overview of different disruption and homogenization methods. The different disruption and homogenization methods listed in Table 4 are described in more detail below.

**Table 4. Disruption and Homogenization Methods**

| <b>Disruption method</b>    | <b>Homogenization method</b> | <b>Comments</b>   |
|-----------------------------|------------------------------|---|
| TissueLyser system          | TissueLyser system           | Simultaneously disrupts and homogenizes up to 192 samples in parallel. The TissueLyser system gives results comparable to using a rotor–stator homogenizer. |
| Rotor–stator homogenization | Rotor–stator homogenization  | Simultaneously disrupts and homogenizes individual samples.   |

## Disruption and homogenization using the QIAGEN TissueLyser system

In bead-milling, tissues can be disrupted by rapid agitation in the presence of beads and lysis buffer. Disruption and simultaneous homogenization occur by the shearing and crushing action of the beads as they collide with the cells. Disruption efficiency is influenced by:

- size and composition of beads
- ratio of buffer to beads
- amount of starting material
- speed and configuration of the TissueLyser
- disintegration time

Stainless steel beads with a diameter of 5 mm are optimal to use for animal tissues in combination with the RNeasy 96 Universal Tissue Kit. All other disruption parameters should be determined empirically for each application. The protocols in this handbook give guidelines for disruption and homogenization of tissues using the TissueLyser and stainless steel beads. For other bead mills, please refer to suppliers' guidelines for further details.

## Disruption and homogenization using rotor–stator homogenizers

Rotor–stator homogenizers thoroughly disrupt and simultaneously homogenize, in the presence of lysis buffer, single samples of animal tissues in 15–90 seconds depending on the toughness and size of the sample. The rotor turns at a very high speed causing the sample to be disrupted and homogenized by a combination of turbulence and mechanical shearing. Foaming of the sample should be kept to a minimum by using properly sized vessels, keeping the tip of the homogenizer submerged, and holding the immersed tip to one side of the tube. Rotor–stator homogenizers are available in different sizes and operate with differently sized probes.

## Square-well blocks

Square-well blocks are supplied with the kit. If several RNeasy 96 plates are processed per day, it may be convenient to keep extra square-well blocks on hand. See ordering information on page 44.

Fresh square-well blocks must be used to take up the aqueous phase. **Do not reuse cleaned square-well blocks to collect the aqueous phase.**

Square-well blocks may be cleaned and reused as waste trays. To reuse the square-well blocks as waste trays, rinse them thoroughly with tap water,\* and incubate for 2 hours or overnight in 0.1 N NaOH, 1 mM EDTA.\* Rinse in distilled water\* and dry at 50°C.

**Note:** Do not use bleach.\* Bleach may react with residual amounts of QIAzol Lysis Reagent and Buffer RW1 on the square-well blocks.

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

# Protocol: Purification of Total RNA from Animal Tissues Using Vacuum/Spin Technology

## Determining the correct amount of starting material

It is essential to begin with the correct amount of tissue in order to obtain optimal RNA yields and purity with RNeasy 96 Universal Tissue plates. Generally, this protocol can be used with a maximum of

- 50 mg flash-frozen tissue
- 100 mg flash-frozen adipose tissue
- 25 mg flash-frozen liver, thymus, or spleen tissue
- 25 mg RNA*later* stabilized tissue

Using fresh tissue is not recommended since RNA in unstabilized fresh tissue is not protected until the sample is homogenized in QIAzol Lysis Reagent. RNA is therefore likely to degrade during the time that it takes to excise 96 tissue samples.

Average RNA yields from various sources are given in Table 3 (page 16).

**Do not overload the plates. Overloading will significantly reduce yields and quality and may cause clogging of the RNeasy 96 Universal Tissue plate.**

## Important points before starting

- If using the RNeasy 96 Universal Tissue Kit for the first time, read “Important Notes” (pages 15–18).
- If preparing RNA for the first time, read Appendix A (pages 33–34).
- Flash-frozen or RNA*later* stabilized tissue can be used. To freeze tissue for long-term storage, flash-freeze in liquid nitrogen,\* and immediately transfer to  $-70^{\circ}\text{C}$ . Tissue can be stored for several months at  $-70^{\circ}\text{C}$ . To process, do not allow tissue to thaw during weighing or handling prior to disruption in QIAzol Lysis Reagent. Homogenized tissue lysates can also be stored at  $-70^{\circ}\text{C}$  for several months. To process frozen homogenized lysates, thaw samples at room temperature or at  $37^{\circ}\text{C}$  in a water bath until they are completely thawed and salts in the QIAzol Lysis Reagent are dissolved. Avoid extended treatment at  $37^{\circ}\text{C}$ , which can cause chemical degradation of RNA. Continue with step 9.

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

- Generally, DNase digestion is not required since integrated QIAzol and RNeasy 96 technologies efficiently remove most of the DNA without DNase treatment. However, further DNA removal may be desirable for certain RNA applications that are sensitive to very small amounts of DNA. In these cases, small residual amounts of DNA remaining can be removed using the optional on-plate DNase digestion or by a DNase digestion after RNA purification (please contact QIAGEN Technical Services for a protocol). For on-plate DNase digestion, prepare the DNase I stock solution as described on page 40 before beginning the procedure.
- QIAzol Lysis Reagent and Buffer RW1 contain a guanidine salt and are therefore not compatible with disinfecting reagents containing bleach. See page 6 for safety information. Take appropriate safety measures and wear gloves when handling.
- Use of a multichannel pipet is recommended (see page 10). Pour buffers and RNase-free water into reagent reservoirs for multichannel pipets. Use reservoirs from a freshly opened package or clean them as described for square-well blocks (see page 18). Make sure that reagent reservoirs used for chloroform are chloroform-resistant.
- A vacuum source capable of generating a vacuum pressure of  $-800$  to  $-900$  mbar is required (see pages 12–14). The vacuum must be switched off and the manifold ventilated between pipetting steps to maintain uniform conditions for each sample.
- All centrifugation steps in the protocol are performed in a Centrifuge 4K15C (see pages 11–12).
- The preliminary centrifugation step (step 9) and the centrifugation step to separate the aqueous from the organic phase (step 12) should be done at  $4^{\circ}\text{C}$ . All other steps of the RNeasy 96 Universal Tissue protocol should be performed at room temperature ( $15$ – $25^{\circ}\text{C}$ ). Avoid interruptions during the procedure.

### Things to do before starting

- Buffer RPE is supplied as a concentrate. Before using for the first time, add 4 volumes of ethanol (96–100%) to obtain a working solution.
- Check that all buffers are at room temperature ( $15$ – $25^{\circ}\text{C}$ ). If using the optional on-plate DNase digestion, see Appendix D, page 40 for details to prepare the DNase I incubation mix.

### Procedure

1. **Preparation of QIAvac 96 vacuum manifold: Place the waste tray inside the QIAvac base. Place the top plate squarely over the base. Place the RNeasy 96 plate in the QIAvac top plate, making sure that the plate is seated tightly. Attach the QIAvac 96 manifold to the vacuum source. Keep vacuum switched off.**

**Note:** Always place the RNeasy 96 plate into the vacuum manifold with the beveled edges pointing to the right-hand side.

- 2. Place 5 mm stainless steel beads into the collection microtubes (1 bead per tube), and transfer the collection microtube rack to a box with dry ice.**

**Note:** We recommend using the TissueLyser for parallel disruption and homogenization of up to 192 samples in parallel. Alternatively a rotor–stator homogenizer can be used for tissue disruption and homogenization. This protocol describes RNA purification from flash-frozen tissue using the TissueLyser. For RNA later stabilized tissue, cooling the collection microtube rack on dry ice is not necessary.

- 3. Remove the tissue sample from RNA later RNA Stabilization Reagent or from cold storage.**

Do not allow the tissue to thaw before it is placed in QIAzol Lysis Reagent.

- 4. Determine the amount of tissue. Do not use more than 50 mg flash-frozen tissue, 25 mg liver, thymus, spleen, or RNA later stabilized tissue, or 100 mg adipose tissue. Transfer it immediately to a cooled collection microtube. Repeat this until all required pieces of tissues are placed in the collection microtubes.**

Weighing tissue is the most accurate way to determine the amount. See pages 15–16 for guidelines to determine the amount of starting material.

RNA in unstabilized tissues is not protected after harvesting until the sample is flash-frozen, or disrupted and homogenized in protocol steps 6 and 7. Frozen animal tissue should not be allowed to thaw during handling. The relevant procedures should be carried out as quickly as possible.

- 5. Remove the collection microtube rack from the dry ice, and immediately pipet 750 µl QIAzol Lysis Reagent into each collection microtube.**
- 6. Close the collection microtube rack using the supplied strips of collection microtube caps, and homogenize on the TissueLyser for 5 min at 25 Hz.**
- 7. Rotate the TissueLyser rack to allow even homogenization, and homogenize for another 5 min at 25 Hz.**

Some exceptionally tough tissues (e.g., pig skin) may not be completely homogenized after 2 x 5 min. This does not affect the protocol, however, since undisrupted pieces of tissue are removed after phase separation.

- 8. Place the collection microtube rack containing the homogenate on the benchtop at room temperature (15–25°C) for 5 min.**
- 9. Load the collection microtube rack into the holder, and place it in the rotor bucket. Centrifuge at 6000 x g for 1 min at 4°C to collect residual liquid from the caps of the tubes.**
- 10. Add 150 µl chloroform. Securely cap the collection microtube rack containing the homogenates using new strips of collection microtube caps, and shake it vigorously while inverting the rack for 15 s.**

Thorough mixing is important for subsequent phase separation.

11. Place the collection microtube rack on the benchtop at room temperature for 2–3 min.
12. Centrifuge at 6,000 x g for 15 min at 4°C. After centrifuging, heat the centrifuge to room temperature if the same centrifuge is to be used for the following centrifugation steps of the protocol.

After centrifugation, the sample separates into 3 phases: an upper, colorless, aqueous phase containing RNA; a white interphase; and a lower, red, organic phase. For tissues with an especially high fat content, an additional, clear phase may be visible below the red, organic phase. The volume of the aqueous phase should be approximately 400 µl.

13. Transfer all of the upper, aqueous phases to a new square-well block. Then add 1 volume (usually 400 µl) of 70% ethanol to each transferred aqueous phase, and mix by pipetting up and down. Do not centrifuge. Continue with step 14.

If some of the aqueous phase is lost during this step, adjust the volume of ethanol accordingly.

14. Pipet the samples (approximately 800 µl) from step 13 into the wells of the RNeasy 96 plate, and switch on the vacuum source. Apply vacuum until transfer is complete (1–5 min). Switch off the vacuum, and ventilate the QIAvac 96 manifold.

Make sure that the QIAvac 96 vacuum manifold is assembled correctly before loading. The flow-through is collected in the waste tray. The vacuum must be switched off and the manifold ventilated between pipetting steps to maintain uniform conditions for each sample.

Take care not to wet the rims of the wells to avoid cross-contamination in subsequent steps

**Note:** Tape unused wells with adhesive tape. Do not use the AirPore Tape Sheets supplied with the RNeasy 96 Universal Tissue Kit. Use either adhesive tape or tape pads (cat. no. 19570) from QIAGEN.

**Optional DNase digest:** Generally, DNase digestion is not required since integrated QIAzol and RNeasy 96 technologies efficiently remove most of the DNA without DNase treatment. However, further DNA removal may be desirable for certain RNA applications that are sensitive to very small amounts of DNA. See Appendix D, pages 40–41, for more information and for details to prepare the DNase I incubation mix.

15. Add 800 µl of Buffer RW1 to each well of the RNeasy 96 plate. Switch on the vacuum source, and apply vacuum until transfer is complete (1–5 min). Switch off the vacuum, and ventilate the QIAvac 96 manifold.

Collect the wash fraction in the same waste tray used in step 14.

16. Lift the top plate carrying the RNeasy 96 plate off the base, and empty the waste tray.\* Reassemble the QIAvac 96 vacuum manifold.
17. Add 800  $\mu$ l of Buffer RPE to each well of the RNeasy 96 plate, and switch on the vacuum source. Apply vacuum until transfer is complete (1–5 min). Switch off the vacuum, and ventilate the QIAvac 96 manifold.

**Note:** Ensure that ethanol is added to Buffer RPE (see “Things to do before starting”, page 20).

18. Place the RNeasy 96 plate on top of a square-well block.
19. Add another 800  $\mu$ l of Buffer RPE to each well of the RNeasy 96 plate. Seal the RNeasy 96 plate with an AirPore Tape Sheet. Load the square-well block and RNeasy 96 plate into the holder, and place the whole assembly in the rotor bucket. Centrifuge at 6000 rpm (approximately 5600  $\times$  g) for 10 min at room temperature to dry the plate membranes.

Centrifugation with sealed plates prevents cross-contamination.

It is important to dry the RNeasy membrane since residual ethanol may interfere with subsequent reactions. The 10 min spin ensures that residual traces of salt are removed and that no ethanol is carried over during elution.

20. Remove the AirPore Tape Sheet. Place the RNeasy 96 plate on top of a clean elution microtube rack containing 0.85 ml elution microtubes.
21. To elute the RNA, add 45–70  $\mu$ l RNase-free water to each well, and seal the RNeasy 96 plate with a new AirPore Tape Sheet. Incubate for 1 min at room temperature. Then centrifuge at 6000 rpm (approximately 5600  $\times$  g) for 4 min at room temperature.

**Note:** Make sure to pipet the RNase-free water directly onto the RNeasy membrane. Elution will be incomplete if some of the water sticks to the walls or the O-rings of the RNeasy 96 plate.

Although eluting with the minimum amount of RNase-free water results in increased RNA concentrations, total yields might be reduced, especially for tissues with low amounts of RNA, such as adipose tissue or skin.

22. Remove the AirPore Tape Sheet. Repeat the elution step (step 21) once with a second volume of 45–70  $\mu$ l RNase-free water.

**Note:** Repeating the elution step is required for complete recovery of RNA.

Use elution microtube caps (caps for strips) provided to seal the microtubes for storage. Store RNA at  $-20^{\circ}\text{C}$  or at  $-70^{\circ}\text{C}$ .

\* Flow-through contains QIAzol Lysis Reagent or Buffer RW1 and is therefore not compatible with bleach. See page 6 for safety information.

# Protocol: Purification of Total RNA from Animal Tissues Using Spin Technology

## Determining the correct amount of starting material

It is essential to begin with the correct amount of tissue in order to obtain optimal RNA yield and purity with RNeasy 96 Universal Tissue plates. Generally, this protocol can be used with a maximum of

- 50 mg flash-frozen tissue
- 100 mg flash-frozen adipose tissue
- 25 mg flash-frozen liver, thymus, or spleen tissue
- 25 mg RNA*later* stabilized tissue

Using fresh tissue is not recommended since RNA in unstabilized fresh tissue is not protected until the sample is homogenized in QIAzol Lysis Reagent. RNA is therefore likely to degrade during the time that it takes to excise 96 tissue samples.

Average RNA yields from various sources are given in Table 3 (page 16).

**Do not overload the plates. Overloading will significantly reduce yield and quality and may cause clogging of the RNeasy 96 Universal Tissue plate.**

## Important points before starting

- If using the RNeasy 96 Universal Tissue Kit for the first time, read “Important Notes” (pages 15–18).
- If preparing RNA for the first time, read Appendix A (pages 33–34).
- Flash-frozen or RNA*later* stabilized tissue can be used. To freeze tissue for long-term storage, flash-freeze in liquid nitrogen,\* and immediately transfer to  $-70^{\circ}\text{C}$ . Tissue can be stored for several months at  $-70^{\circ}\text{C}$ . To process, do not allow tissue to thaw during weighing or handling prior to disruption in QIAzol Lysis Reagent. Homogenized tissue lysates can also be stored at  $-70^{\circ}\text{C}$  for several months. To process frozen homogenized lysates, thaw samples at room temperature or at  $37^{\circ}\text{C}$  in a water bath until they are completely thawed and salts in the lysis buffer are dissolved. Avoid extended treatment at  $37^{\circ}\text{C}$ , which can cause chemical degradation of the RNA. Continue with step 8.

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.



- Generally, DNase digestion is not required since integrated QIAzol and RNeasy 96 technologies efficiently remove most of the DNA without DNase treatment. However, further DNA removal may be desirable for certain RNA applications that are sensitive to very small amounts of DNA. In these cases, small residual amounts of DNA remaining can be removed using the optional on-plate DNase digestion or by a DNase digestion after RNA purification (please contact QIAGEN Technical Services for a protocol). For on-plate DNase digestion, prepare the DNase I stock solution as described on page 40 before beginning the procedure.
- QIAzol Lysis Reagent and Buffer RW1 contain a guanidine salt and are therefore not compatible with disinfecting reagents containing bleach. See page 6 for safety information. Take appropriate safety measures and wear gloves when handling.
- Use of a multichannel pipet is recommended (see page 10). Pour buffers and RNase-free water into reagent reservoirs for multichannel pipets. Use reservoirs from a freshly opened package or clean them as described for square-well blocks (see page 18). Make sure that reagent reservoirs used for chloroform are chloroform-resistant.
- All centrifugation steps in the protocol are performed in a Centrifuge 4K15C (see pages 11–12).
- The preliminary centrifugation step (step 8) and the centrifugation step to separate the aqueous from the organic phase (step 11) should be done at 4°C. All other steps of the RNeasy 96 Universal Tissue protocol should be performed at room temperature (15–25°C). Avoid interruptions during the procedure.

### Things to do before starting

- Buffer RPE is supplied as a concentrate. Before using for the first time, add 4 volumes of ethanol (96–100%) to obtain a working solution.
- Check that all buffers are at room temperature (15–25°C). If using the optional on-plate DNase digestion, see Appendix D, page 40 for details to prepare the DNase I incubation mix.

### Procedure

- 1. Place 5 mm stainless steel beads into the collection microtubes (1 bead per tube), and transfer the collection microtube rack to a box with dry ice.**

**Note:** We recommend using the TissueLyser for parallel disruption and homogenization of up to 192 samples in parallel. Alternatively a rotor–stator homogenizer can be used for tissue disruption and homogenization. This protocol describes RNA purification from flash-frozen tissue using the TissueLyser. For RNAlater stabilized tissue, cooling the collection microtube rack on dry ice is not necessary.

2. **Remove the tissue sample from RNA<sup>later</sup> RNA Stabilization Reagent or from cold storage.**

Do not allow the tissue to thaw before it is placed in QIAzol Lysis Reagent.

3. **Determine the amount of tissue. Do not use more than 50 mg flash-frozen tissue, 25 mg liver, thymus, spleen, or RNA<sup>later</sup> stabilized tissue, or 100 mg adipose tissue. Transfer it immediately to a cooled collection microtube. Repeat this until all required pieces of tissues are placed in the collection microtubes.**

Weighing tissue is the most accurate way to determine the amount. See pages 15–16 for guidelines to determine the amount of starting material.

RNA in unstabilized tissues is not protected after harvesting until the sample is flash-frozen, or disrupted and homogenized in protocol steps 5 and 6. Frozen animal tissue should not be allowed to thaw during handling. The relevant procedures should be carried out as quickly as possible

4. **Remove the collection microtube rack from the dry ice, and immediately pipet 750  $\mu$ l QIAzol Lysis Reagent into each collection microtube.**
5. **Close the collection microtube rack using the supplied strips of collection microtube caps and homogenize on the TissueLyser for 5 min at 25 Hz.**
6. **Rotate the TissueLyser rack to allow even homogenization, and homogenize for another 5 min at 25 Hz.**

Some exceptionally tough tissues (e.g., pig skin) may not be completely homogenized after 2 x 5 min. This does not affect the protocol, however, since undisrupted pieces of tissue are removed after phase separation.

7. **Place the collection microtube rack containing the homogenate on the benchtop at room temperature (15–25°C) for 5 min.**
8. **Load the collection microtube rack into the holder, and place it in the rotor bucket. Centrifuge at 6000 x g for 1 min at 4°C to collect residual liquid from the caps of the tubes.**
9. **Add 150  $\mu$ l chloroform. Securely cap the collection microtube rack containing the homogenates using new strips of collection microtube caps, and shake it vigorously while inverting the rack for 15 s.**

Thorough mixing is important for subsequent phase separation.

10. **Place the collection microtube rack on the benchtop at room temperature for 2–3 min.**

- 11. Centrifuge at 6,000 x g for 15 min at 4°C. After centrifuging, heat the centrifuge to room temperature if the same centrifuge is to be used for the following centrifugation steps of the protocol.**

After centrifugation, the sample separates into 3 phases: an upper, colorless, aqueous phase containing RNA; a white interphase; and a lower, red, organic phase. For tissues with an especially high fat content, an additional, clear phase may be visible below the red, organic phase. The volume of the aqueous phase should be approximately 400  $\mu$ l.

- 12. Transfer all of the upper, aqueous phases to a new square-well block. Then add 1 volume (usually 400  $\mu$ l) of 70% ethanol to each transferred aqueous phase, and mix by pipetting up and down. Do not centrifuge. Continue with step 13.**

If some of the aqueous phase is lost during this step, adjust the volume of ethanol accordingly.

- 13. Place an RNeasy 96 plate on top of a square-well block.**
- 14. Pipet the samples (approximately 800  $\mu$ l) from step 12 into the wells of the RNeasy 96 plate.**

Take care not to wet the rims of the wells to avoid cross-contamination in subsequent steps.

- 15. Seal the RNeasy 96 plate with an AirPore Tape Sheet. Load the square-well block and RNeasy 96 plate into the holder, and place the whole assembly in the rotor bucket. Centrifuge at 6000 rpm (approximately 5600 x g) for 4 min at room temperature.**

Centrifugation with sealed plates prevents cross-contamination.

**Optional DNase digestion:** Generally, DNase digestion is not required since integrated QIAzol and RNeasy 96 technologies efficiently remove most of the DNA without DNase treatment. However, further DNA removal may be desirable for certain RNA applications that are sensitive to very small amounts of DNA. See Appendix D, pages 40–41, for more information and for details to prepare the DNase I incubation mix.

- 16. Empty the square-well block,\* and remove the AirPore Tape Sheet. Add 800  $\mu$ l of Buffer RW1 to each well of the RNeasy 96 plate. Seal the RNeasy 96 plate with a new AirPore Tape Sheet. Centrifuge at 6000 rpm (approximately 5600 x g) for 4 min at room temperature.**

\* Flow-through contains QIAzol Lysis Reagent or Buffer RW1 and is therefore not compatible with bleach. See page 6 for safety information.

17. Empty the square-well block,\* and remove the AirPore Tape Sheet. Add 800  $\mu$ l Buffer RPE to each well of the RNeasy 96 plate. Seal the RNeasy 96 plate with a new AirPore Tape Sheet. Centrifuge at 6000 rpm (approximately 5600 x g) for 4 min at room temperature.

**Note:** Ensure that ethanol is added to Buffer RPE (see “Things to do before starting”, page 25).

18. Empty the square-well block, and remove the AirPore Tape Sheet. Add another 800  $\mu$ l Buffer RPE to each well of the RNeasy 96 plate. Seal the RNeasy 96 plate with a new AirPore Tape Sheet. Centrifuge at 6000 rpm (approximately 5600 x g) for 10 min at room temperature.

It is important to dry the RNeasy membrane since residual ethanol may interfere with subsequent reactions. The 10 min spin ensures that residual traces of salt are removed and that no ethanol is carried over during elution.

19. Remove AirPore Tape Sheet. Place the RNeasy 96 plate on top of a clean elution microtube rack containing 0.85 ml elution microtubes.
20. To elute the RNA, add 45–70  $\mu$ l of RNase-free water to each well, and seal the RNeasy 96 plate with a new AirPore Tape Sheet. Incubate for 1 min at room temperature. Then centrifuge at 6000 rpm (approximately 5600 x g) for 4 min at room temperature.

**Note:** Make sure to pipet the RNase-free water directly onto the RNeasy membrane. Elution will be incomplete if some of the water sticks to the walls or the O-rings of the RNeasy 96 plate.

Although eluting with the minimum amount of RNase-free water results in increased RNA concentrations, total yields might be reduced, especially for tissues with low amounts of RNA, such as adipose tissue or skin.

21. Remove the AirPore Tape Sheet. Repeat the elution step (step 20) once with a second volume of 45–70  $\mu$ l RNase-free water.

**Note:** Repeating the elution step is required for complete recovery of RNA.

Use elution microtube caps (caps for strips) provided to seal the microtubes for storage. Store RNA at  $-20^{\circ}\text{C}$  or at  $-70^{\circ}\text{C}$ .

\* Flow-through contains QIAzol Lysis Reagent or Buffer RW1 and is therefore not compatible with bleach. See page 6 for safety information.

# Troubleshooting Guide

This troubleshooting guide may be helpful in solving any problems that may arise. The scientists in QIAGEN Technical Services are always happy to answer any questions you may have about either the information and protocols in this handbook or molecular biology applications (see back cover for contact information).

## Comments and suggestions

---

### Phases do not separate completely

- |    |   |  |
|----|---|--|
| a) | No chloroform added or chloroform not pure              | Make sure to add chloroform that does not contain isoamyl alcohol or other additives.  |
| b) | Homogenate not sufficiently mixed before centrifugation | After addition of chloroform (vacuum/spin step 10; spin step 9), the homogenate must be vigorously shaken. If the phases are not well separated, shake the rack vigorously while inverting it for at least 15 s, and repeat the incubation and centrifugation (vacuum/spin steps 11 and 12, page 22; spin steps 10 and 11, pages 26–27). |
| c) | Organic solvents in samples used for purification       | Make sure that the starting sample does not contain organic solvents (e.g., ethanol, DMSO), strong buffers, or alkaline reagents.* These can interfere with the phase separation.  |

### Clogged plate wells

- |    |  |  |
|----|--|--|
| a) | Inefficient disruption and/or homogenization | See “Disruption and homogenization of starting materials” (pages 17–18) for a detailed description of disruption and homogenization methods.   |
| b) | Too much starting material                   | Reduce amount of starting material. It is essential not to exceed the maximum amount of starting material (see pages 15–16).   |
| c) | Centrifugation temperature too low           | Except for phase separation, all centrifugation steps should be performed at room temperature (15–25°C). Some centrifuges may cool to below 20°C even when set at 20°C. This can cause precipitates to form that can clog the RNeasy 96 plate. If this happens, set the centrifugation temperature to 25°C, and warm the ethanol-containing lysate to 37°C before transferring to the RNeasy 96 plate. |

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

## Comments and suggestions

---

### Little or no RNA eluted

- |                                    |  |
|------------------------------------|--|
| a) Too much starting material      | Overloading significantly reduces yield. Reduce the amount of starting material (see pages 15–16).   |
| b) Buffer temperatures too low     | All buffers must be at room temperature (15–25°C) throughout the procedure.  |
| c) RNA still bound to the membrane | Repeat elution, but incubate the RNeasy 96 plate on the benchtop at room temperature for 10 min with RNase-free water before centrifuging. |

### Low $A_{260}/A_{280}$ value

- |   |  |
|---|--|
| a) Not enough QIAzol Lysis Reagent used for homogenization    | In subsequent preparations, reduce the amount of starting material and/or increase the volume of QIAzol Lysis Reagent and the homogenization time. |
| b) Sample not incubated for 5 min after homogenization        | Place the sample at room temperature (15–25°C) for 5 min after homogenization, as indicated in the protocol.                                       |
| c) Water used to dilute RNA for $A_{260}/A_{260}$ measurement | Use 10 mM Tris·Cl, * pH 7.5, not RNase-free water, to dilute the sample before measuring purity (see “Purity of RNA”, page 36).                    |

### RNA degraded

- |  |   |
|--|---|
| a) Inappropriate handling of starting material | Ensure that tissues have been properly handled and that the protocol has been performed without interruptions, especially the initial steps involving tissue lysis and homogenization. Some tissues (e.g., pancreas or intestine) contain high amounts of RNases. Care must be taken to excise these tissue from animals as fast as possible and to stabilize them either by freezing in liquid nitrogen* or by immersing them in RNA <sup>later</sup> RNA Stabilization Reagent† immediately after excision. |
|--|---|

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

† See the RNA<sup>later</sup> Handbook for more information about RNA<sup>later</sup> RNA Stabilization Reagent.

## Comments and suggestions

---

- b) RNase contamination      Check for RNase contamination of buffers. Although all buffers have been tested and are guaranteed RNase-free, RNases can be introduced during use. Be certain not to introduce any RNases during the procedure or later handling. See Appendix A (pages 33–34) for general remarks on handling RNA.

### DNA contamination in downstream experiments

- a) Phase separation performed at too high a temperature      The phase separation should be performed at 4°C to allow optimal phase separation and removal of genomic DNA from the aqueous phase. Make sure that the centrifuge does not heat above 10°C during the centrifugation.
- b) Interphase contamination of aqueous phase      Contamination of the aqueous phase with the interphase results in an increased DNA content in the eluate. Make sure to transfer the aqueous phase without interphase contamination.
- c) No DNase treatment      Follow the optional on-plate DNase digestion using the RNase-Free DNase Set (Appendix D, pages 40–41) at the point indicated in the protocol.  
  
Alternatively, after the RNeasy procedure, DNase digest the eluate containing the RNA. After inactivating DNase by heat treatment, the RNA can be either used directly in the subsequent application without further treatment, or repurified using an RNeasy RNA cleanup protocol (see the *RNeasy 96 Handbook* or the *RNeasy MinElute™ Cleanup Handbook*).

### RNA concentration too low

- Elution volume too high      Elute with less RNase-free water. Although eluting with less RNase-free water results in increased RNA concentrations, total yields might be reduced, especially for tissues with low amounts of RNA, such as adipose tissue or skin.

## Comments and suggestions

---

### RNA does not perform well in downstream experiments

- a) Salt carryover during elution      Ensure that Buffer RPE is at room temperature (15–25°C).
- b) Ethanol carryover      During the second Buffer RPE wash, be sure to dry the plate-well membranes by centrifuging the plate at 6000 rpm (approximately 5600 x g) for 10 min at room temperature.
- c) Vacuum/spin protocol: Vacuum pressure too low      A vacuum source capable of generating a vacuum pressure of –800 to –900 mbar is necessary to achieve efficient RNA binding to the membrane and washing.

### Low well-to-well reproducibility

- a) Elution volume too low      Use elution volumes of 2 x 50 or 2 x 70 µl to improve well-to-well reproducibility.
- b) Vacuum pressure too low      A vacuum source capable of generating a vacuum pressure of –800 to –900 mbar is necessary to achieve efficient RNA binding to the membrane and washing.
- c) Incomplete homogenization      Some types of tissues are more difficult to homogenize, resulting in greater variability from sample to sample.
- d) Variability between samples      RNA yields from tissue samples can vary more than, for example, cultured cells due to the heterogeneous nature of most tissues and donor-to-donor variability.



# Appendix A: General Remarks on Handling RNA

## Handling RNA

Ribonucleases (RNases) are very stable and active enzymes that generally do not require cofactors to function. Since RNases are difficult to inactivate and even minute amounts are sufficient to destroy RNA, do not use any plasticware or glassware without first eliminating possible RNase contamination. Great care should be taken to avoid inadvertently introducing RNases into the RNA sample during or after the purification procedure. In order to create and maintain an RNase-free environment, the following precautions must be taken during pretreatment and use of disposable and non-disposable vessels and solutions while working with RNA.

### General handling

Proper microbiological, aseptic technique should always be used when working with RNA. Hands and dust particles may carry bacteria and molds and are the most common sources of RNase contamination. Always wear latex or vinyl gloves while handling reagents and RNA samples to prevent RNase contamination from the surface of the skin or from dusty laboratory equipment. Change gloves frequently and keep tubes closed whenever possible. Keep purified RNA on ice\* when aliquots are pipetted for downstream applications.

### Disposable plasticware

The use of sterile, disposable polypropylene tubes is recommended throughout the procedure. These tubes are generally RNase-free and do not require pretreatment to inactivate RNases. For sensitive downstream applications, the use of filter tips is recommended in order to avoid cross contamination.

### Non-disposable plasticware

Non-disposable plasticware should be treated before use to ensure that it is RNase-free. Plasticware should be thoroughly rinsed with 0.1 M NaOH, 1 mM EDTA\* followed by RNase-free water (see "Solutions", page 34). Alternatively, chloroform-resistant plasticware can be rinsed with chloroform to inactivate RNases.

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

## Glassware

Glassware should be treated before use to ensure that it is RNase-free. Glassware used for RNA work should be cleaned with a detergent,\* thoroughly rinsed, and oven baked at 240°C for 4 or more hours (overnight, if more convenient) before use. Autoclaving alone will not fully inactivate many RNases. Alternatively, glassware can be treated with DEPC\* (diethyl pyrocarbonate). Fill glassware with 0.1% DEPC (0.1% in water), allow to stand overnight (12 hours) at 37°C, and then autoclave or heat to 100°C for 15 minutes to eliminate residual DEPC.

## Electrophoresis tanks

Electrophoresis tanks should be cleaned with detergent solution (e.g., 0.5% SDS),\* thoroughly rinsed with RNase-free water, and then rinsed with ethanol<sup>†</sup> and allowed to dry.

## Solutions

Solutions (water and other solutions)\* should be treated with 0.1% DEPC. DEPC is a strong, but not absolute, inhibitor of RNases. It is commonly used at a concentration of 0.1% to inactivate RNases on glass or plasticware or to create RNase-free solutions and water. DEPC inactivates RNases by covalent modification. Add 0.1 ml DEPC to 100 ml of the solution to be treated and shake vigorously to bring the DEPC into solution. Let the solution incubate for 12 hours at 37°C. Autoclave for 15 minutes to remove any trace of DEPC. DEPC will react with primary amines and cannot be used directly to treat Tris buffers.\* DEPC is highly unstable in the presence of Tris buffers and decomposes rapidly into ethanol and CO<sub>2</sub>. When preparing Tris buffers, treat water with DEPC first, and then dissolve Tris to make the appropriate buffer. Trace amounts of DEPC will modify purine residues in RNA by carbethoxylation. Carbethoxylated RNA is translated with very low efficiency in cell-free systems. However, its ability to form DNA:RNA or RNA:RNA hybrids is not seriously affected unless a large fraction of the purine residues have been modified. Residual DEPC must always be eliminated from solutions or vessels by autoclaving or heating to 100°C for 15 minutes.

**Note:** RNeasy buffers are guaranteed RNase-free without using DEPC treatment and are therefore free of any DEPC contamination.

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

<sup>†</sup> Plastics used for some electrophoresis tanks are not resistant to ethanol. Take proper care and check the supplier's instructions.

# Appendix B: Storage, Quantification, and Determination of Quality of RNA

## Storage of RNA

Purified RNA may be stored at  $-20^{\circ}\text{C}$  or  $-70^{\circ}\text{C}$  in RNase-free water. Under these conditions, no degradation of RNA is detectable after 1 year.

## Quantification of RNA

The concentration of RNA should be determined by measuring the absorbance at 260 nm ( $A_{260}$ ) in a spectrophotometer (see "Spectrophotometric quantification of RNA" below). For small amounts of RNA, however, it may be difficult to determine amounts photometrically. Small amounts of RNA can be accurately quantified using an Agilent 2100 bioanalyzer, quantitative RT-PCR, or fluorometric quantification.

## Spectrophotometric quantification of RNA

To ensure significance,  $A_{260}$  readings should be greater than 0.15. An absorbance of 1 unit at 260 nm corresponds to 44  $\mu\text{g}$  of RNA per milliliter ( $A_{260}=1 \Rightarrow 44 \mu\text{g/ml}$ ). This relation is valid only for measurements at a neutral pH. Therefore, if it is necessary to dilute the RNA sample, this should be done in a buffer with neutral pH.\* As discussed below (see "Purity of RNA", page 36), the ratio between the absorbance values at 260 and 280 nm gives an estimate of RNA purity.

When measuring RNA samples, be certain that cuvettes are RNase-free, especially if the RNA is to be recovered after spectrophotometry. This can be accomplished by washing cuvettes with 0.1 M NaOH, 1 mM EDTA,\* followed by washing with RNase-free water (see "Solutions", page 34). Use the buffer in which the RNA is diluted to zero the spectrophotometer. An example of the calculation involved in RNA quantification is shown below:

Volume of RNA sample = 100  $\mu\text{l}$

Dilution = 10  $\mu\text{l}$  of RNA sample + 490  $\mu\text{l}$  of 10 mM Tris-Cl,\* pH 7.0 (1/50 dilution).

Measure absorbance of diluted sample in a 1 ml cuvette (RNase-free).

$A_{260} = 0.20$

Concentration of RNA sample = 44  $\mu\text{g/ml}$   $\times$   $A_{260}$   $\times$  dilution factor  
= 44  $\mu\text{g/ml}$   $\times$  0.20  $\times$  50  
= 440  $\mu\text{g/ml}$

Total amount = concentration  $\times$  volume in milliliters  
= 440  $\mu\text{g/ml}$   $\times$  0.1 ml  
= 44  $\mu\text{g}$  of RNA

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

## Purity of RNA

The ratio of the readings at 260 nm and 280 nm ( $A_{260}/A_{280}$ ) provides an estimate of the purity of RNA with respect to contaminants that absorb in the UV spectrum, such as protein. However, the  $A_{260}/A_{280}$  ratio is influenced considerably by pH. Since water is not buffered, the pH and the resulting  $A_{260}/A_{280}$  ratio can vary greatly. Lower pH results in a lower  $A_{260}/A_{280}$  ratio and reduced sensitivity to protein contamination.\* For accurate values, we recommend measuring absorbance in 10 mM Tris-Cl, pH 7.5. Pure RNA has an  $A_{260}/A_{280}$  ratio of 1.9–2.1<sup>†</sup> in 10 mM Tris-Cl, pH 7.5. Always be sure to calibrate the spectrophotometer with the same solution used for dilution.

For determination of RNA concentration, however, we recommend dilution of the sample in a buffer with neutral pH since the relationship between absorbance and concentration ( $A_{260}$  reading of 1 = 44  $\mu\text{g}/\text{ml}$  RNA) is based on an extinction coefficient calculated for RNA at neutral pH (see “Spectrophotometric quantification of RNA”, page 35).

## DNA contamination

No currently available purification method can guarantee that RNA is completely free of DNA, even when it is not visible on an agarose gel. To prevent any interference by DNA in RT-PCR applications, such as ABI PRISM<sup>®</sup> and LightCycler<sup>®</sup> RT-PCR analyses, we recommend designing primers<sup>‡</sup> that anneal at intron splice junctions so that genomic DNA will not be amplified. Alternatively, DNA contamination can be detected on agarose gels<sup>‡</sup> following RT-PCR by performing control experiments in which no reverse transcriptase<sup>‡</sup> is added prior to the PCR step or by using intron-spanning primers. For sensitive applications, such as differential display, or if it is not practical to use splice-junction primers, DNase digestion of the purified RNA with RNase-free DNase<sup>‡</sup> is recommended.

A protocol for optional on-plate DNase digestion using the RNase-Free DNase Set is provided in Appendix D (pages 40–41). The DNase is efficiently washed away in the subsequent wash steps. Alternatively, after the RNeasy procedure, the eluate containing the RNA can be treated with DNase (please contact QIAGEN Technical Service for a protocol). The RNA can then be repurified using an RNeasy RNA cleanup protocol (see the *RNeasy 96 Handbook* or the *RNeasy MinElute Cleanup Handbook*), or after heat inactivation of the DNase, the RNA can be used directly in downstream applications.

\* Wilfinger, W.W., Mackey, M., and Chomczynski, P. (1997) Effect of pH and ionic strength on the spectrophotometric assessment of nucleic acid purity. *BioTechniques* **22**, 474.

<sup>†</sup> Values up to 2.3 are routinely obtained for pure RNA (in 10 mM Tris-Cl, pH 7.5) with some spectrophotometers.

<sup>‡</sup> When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

## Integrity of RNA

The integrity and size distribution of total RNA purified with RNeasy Kits can be checked by denaturing agarose gel electrophoresis and ethidium bromide\* staining or using an Agilent 2100 bioanalyzer. The respective ribosomal RNAs should appear as sharp bands or peaks. The apparent ratio of 28S rRNA to 18S RNA should be approximately 2:1. If the ribosomal bands or peaks of a specific sample are not sharp, but appear as a smear towards smaller sized RNAs, it is likely that the RNA sample suffered major degradation during preparation.

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

## Appendix C: Protocol for Formaldehyde Agarose Gel Electrophoresis

The following protocol for formaldehyde agarose (FA) gel electrophoresis is routinely used at QIAGEN and gives enhanced sensitivity for gel and subsequent analysis (e.g., northern blotting). A key feature is the concentrated RNA loading buffer that allows a larger volume of RNA sample to be loaded onto the gel than conventional protocols (e.g., Sambrook et al., eds. [1989] *Molecular cloning — a laboratory manual*, 2nd ed. Cold Spring Harbor, NY: Cold Spring Harbor Laboratory Press).

### FA gel preparation

To prepare FA gel (1.2% agarose) of size 10 x 14 x 0.7 cm, mix:

|       |   |
|-------|---|
| 1.2 g | agarose*                                  |
| 10 ml | 10x FA gel buffer (see composition below) |

add RNase-free water to 100 ml

If smaller or larger gels are needed, adjust the quantities of components proportionately. Heat the mixture to melt agarose. Cool to 65°C in a water bath. Add 1.8 ml of 37% (12.3 M) formaldehyde\* and 1 µl of a 10 mg/ml ethidium bromide\* stock solution. Mix thoroughly and pour onto gel support. Prior to running the gel, equilibrate in 1x FA gel running buffer (see composition below) for at least 30 min.

### RNA sample preparation for FA gel electrophoresis

Add 1 volume of 5x RNA loading buffer (see composition below) to 4 volumes of RNA sample (for example 10 µl of loading buffer and 40 µl of RNA) and mix.

Incubate for 3–5 min at 65°C, chill on ice,\* and load onto the equilibrated FA gel.

### Gel running conditions

Run gel at 5–7 V/cm in 1x FA gel running buffer.

### Composition of FA gel buffers

#### 10x FA gel buffer

|                      |  |
|----------------------|--|
| 200 mM               | 3-[N-morpholino]propanesulfonic acid (MOPS) (free acid)* |
| 50 mM                | sodium acetate*  |
| 10 mM                | EDTA*  |
| pH to 7.0 with NaOH* |  |

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

### 1x FA gel running buffer

|        |                           |
|--------|---------------------------|
| 100 ml | 10x FA gel buffer         |
| 20 ml  | 37% (12.3 M) formaldehyde |
| 880 ml | RNase-free water          |

### 5x RNA loading buffer

|             |   |
|-------------|---|
| 16 $\mu$ l  | saturated aqueous bromophenol blue solution* <sup>†</sup> |
| 80 $\mu$ l  | 500 mM EDTA, pH 8.0                                       |
| 720 $\mu$ l | 37% (12.3 M) formaldehyde                                 |
| 2 ml        | 100% glycerol*  |
| 3.084 ml    | formamide*  |
| 4 ml        | 10x FA gel buffer   |

RNase-free water to 10 ml

Stability: approximately 3 months at 4°C

\* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

<sup>†</sup> To make a saturated solution, add solid bromophenol blue to distilled water. Mix and continue to add more bromophenol blue until no more will dissolve. Centrifuge to pellet the undissolved powder, and carefully pipet the saturated supernatant.

## Appendix D: Optional On-Plate DNase Digestion with the RNase-Free DNase Set

The RNase-Free DNase Set (cat. no. 79254) provides efficient on-plate digestion of DNA during RNA purification. The DNase is efficiently removed in subsequent wash steps.

**Note:** Standard DNase buffers are not compatible with on-plate DNase digestion. Use of other buffers may affect the binding of the RNA to the RNeasy silica-gel membrane, reducing the yield and integrity of the RNA.

Lysis and homogenization of the sample and binding of RNA to the silica-gel membrane are performed according to the standard protocols. After washing with a reduced volume of Buffer RW1, the RNA is treated with DNase I while bound to the silica-gel membrane. The DNase is removed by a second wash with Buffer RW1. Washing with Buffer RPE and elution are then performed according to the standard protocols.

### Important points before starting

- Generally, DNase digestion is not required since integrated QIAzol and RNeasy 96 technologies efficiently remove most of the DNA without DNase treatment. However, further DNA removal may be necessary for certain RNA applications that are sensitive to very small amounts of DNA (e.g., QuantiTect RT-PCR analysis with a low-abundance target). DNA can also be removed by a DNase digestion following RNA purification.
- **Do not vortex the reconstituted DNase I.** DNase I is especially sensitive to physical denaturation. Mixing should only be carried out by gently inverting the tube.
- If desired, these DNase digestion steps can be carried out on the QIAvac 96 vacuum manifold instead of using centrifugation. Please contact QIAGEN Technical Services for more information.

### Things to do before starting

- Prepare DNase I stock solution before using the RNase-Free DNase Set for the first time. The RNeasy 96 Universal Tissue procedure requires 2 RNase-Free DNase Sets per 96-well plate. Dissolve 2 vials of solid DNase I (2 x 1500 Kunitz units) in 2 x 550 µl of the RNase-free water provided. Take care that no DNase I is lost when opening the vial. Mix gently by inverting the tube. Do not vortex.
- Unused DNase I stock solution can be stored at -20°C for up to 9 months. Thawed stock solution can be stored at 2–8°C for up to 6 weeks. Do not refreeze the DNase I stock solution after thawing.



## Procedure

Carry out steps 1–14 in the vacuum/spin protocol or 1–15 of the spin protocol. Instead of continuing with the next Buffer RW1 wash step, follow steps D1–D4 below. If the vacuum/spin protocol is used, centrifugation in steps D1–D4 can be replaced by processing on the QIAvac 96.

**D1. Pipet 400  $\mu$ l Buffer RW1 into each well of the RNeasy 96 plate, and centrifuge at room temperature (15–25°C) for 4 min at 6000 rpm (approximately 5600 g) to wash. Discard the flow-through.\***

Reuse the square-well block in step D3.

**D2. Add 670  $\mu$ l DNase I stock solution (see above) to 7.3 ml Buffer RDD. Mix by gently inverting the tube.**

Buffer RDD is supplied with the RNase-Free DNase Set.

**Note:** DNase I is especially sensitive to physical denaturation. Mixing should only be carried out by gently inverting the tube. Do not vortex.

**D3. Pipet the DNase I incubation mix (80  $\mu$ l per well) directly onto the RNeasy silica-gel membrane in each well of the RNeasy 96 plate, and place on the benchtop at room temperature for 15 min.**

**Note:** Make sure to pipet the DNase I incubation mix directly onto the RNeasy silica-gel membrane. DNase digestion will be incomplete if part of the mix sticks to the walls or the O-ring of the RNeasy 96 plate wells.

**D4. Pipet 400  $\mu$ l Buffer RW1 into each well of the RNeasy 96 plate, and centrifuge for 4 min at 6000 rpm (approximately 5600 g). Discard the flow-through.\* Continue with step 16 of the vacuum/spin protocol (page 23) or step 17 of the spin protocol (page 28).**

\* Flow-through contains Buffer RW1 and is therefore not compatible with bleach. See page 6 for safety information.

## References

QIAGEN maintains a large, up-to-date online database of scientific publications utilizing QIAGEN products. Comprehensive search options allow you to find the articles you need, either by a simple keyword search or by specifying the application, research area, title, etc.

For a complete list of references, visit the QIAGEN Reference Database online at [www.qiagen.com/RefDB/search.asp](http://www.qiagen.com/RefDB/search.asp) or contact QIAGEN Technical Services or your local distributor.

### Quantitative RT-PCR

The application guide *Critical Factors for Successful Real-Time PCR* provides background information, tips, and comprehensive practical guidelines to help get the most out of gene expression analyses. Contact QIAGEN Technical Services or your local distributor for a copy.

# Ordering Information

| Product                                  | Contents   | Cat. no. |
|--|--|----------|
| RNeasy 96 Universal Tissue Kit (4)*      | For 4 x 96 total RNA preps:<br>4 RNeasy 96 Plates, Collection Microtubes (racked), Elution Microtubes CL (0.85 ml), Caps, Square-Well Blocks, AirPore Tape Sheets, RNase-Free Reagents and Buffers   | 74881    |
| RNeasy 96 Universal Tissue Kit (12)*     | For 12 x 96 total RNA preps:<br>12 RNeasy 96 Plates, Collection Microtubes (racked), Elution Microtubes CL (0.85 ml), Caps, Square-Well Blocks, AirPore Tape Sheets, RNase-Free Reagents and Buffers | 74882    |
| <b>Accessories</b>                       |  |          |
| TissueLyser                              | Universal laboratory mixer-mill disruptor  | Inquire  |
| TissueLyser Adapter Set 2 x 96           | 2 sets of Adapter Plates, for use with collection microtubes (racked, 1.2 ml) on the TissueLyser   | 69984    |
| Stainless Steel Beads, 5 mm (200)        | Stainless Steel Beads, suitable for use with 1.2 ml collection microtubes and 2.0 ml microcentrifuge tubes on the TissueLyser  | 69989    |
| TissueLyser 5 mm Bead Dispenser, 96-well | For dispensing 96 beads (5 mm diameter) in parallel  | 69975    |
| Centrifuge 4K15C <sup>†</sup>            | Universal refrigerated laboratory centrifuge with brushless motor  | Inquire  |
| Plate Rotor 2 x 96 <sup>‡</sup>          | Rotor for 2 QIAGEN 96 plates, for use with QIAGEN Centrifuges  | 81031    |

\* Requires use of the Plate Rotor 2 x 96 and Centrifuge 4K15C (QIAvac 96 optional).

<sup>†</sup> Centrifuge 4K15C is not available in all countries. Specific formats are available in Japan. Please inquire.

<sup>‡</sup> The Plate Rotor 2 x 96 is available exclusively from QIAGEN and its distributors. Under the current liability and warranty conditions, the rotor may only be used in Centrifuges 4-15, 4-15C, and 4K15C from QIAGEN and freely programmable models of centrifuges 4-15, 4K15, 6-10, 6K10, 6-15, and 6K15 from Sigma Laborzentrifugen GmbH.

## Ordering Information

| Product   | Contents   | Cat. no. |
|---|--|----------|
| QIAvac 96   | Vacuum manifold for processing QIAGEN 96-well plates: includes QIAvac 96 Top Plate, Base, Waste Tray, Plate Holder, Rack of Collection Microtubes (1.2 ml) | 19504    |
| Vacuum Regulator  | For use with QIAvac manifolds  | 19530    |
| RNase-Free DNase Set (50)                               | 1500 units RNase-Free DNase I, RNase-Free Buffer RDD, and RNase-Free Water for 50 RNA minipreps  | 79254    |
| QIAzol Lysis Reagent (200 ml)                           | 200 ml QIAzol Lysis Reagent  | 79306    |
| RNA <sup>later</sup> RNA Stabilization Reagent (50 ml)  | 50 ml RNA <sup>later</sup> RNA Stabilization Reagent for stabilization of RNA in 25 x 200 mg tissue samples  | 76104    |
| RNA <sup>later</sup> RNA Stabilization Reagent (250 ml) | 250 ml RNA <sup>later</sup> RNA Stabilization Reagent for stabilization of RNA in 125 x 200 mg tissue samples  | 76106    |
| RNA <sup>later</sup> TissueProtect Tubes (50 x 1.5 ml)  | For stabilization of RNA in 50 x 150 mg tissue samples: 50 screw-top tubes containing 1.5 ml RNA <sup>later</sup> RNA Stabilization Reagent each           | 76154    |
| RNA <sup>later</sup> TissueProtect Tubes (20 x 5 ml)    | For stabilization of RNA in 20 x 500 mg tissue samples: 20 screw-top tubes containing 5 ml RNA <sup>later</sup> RNA Stabilization Reagent each             | 76163    |
| Square-Well Blocks (24)                                 | 96-well blocks with 2.2 ml wells, 24 per case  | 19573    |
| AirPore Tape Sheets (50)                                | Microporous tape sheets for covering 96-well blocks: 50 sheets per pack  | 19571    |

“RNA<sup>later</sup>™” is a trademark of AMBION, Inc., Austin, Texas and is covered by various U.S. and foreign patents.

## Ordering Information

| Product                         | Contents  | Cat. no. |
|---------------------------------|---|----------|
| Tape Pads (5)                   | Adhesive tape sheets for sealing multiwell plates and blocks:<br>25 sheets per pad, 5 pads per pack   | 19570    |
| Elution Microtubes CL (24 x 96) | Nonsterile polypropylene tubes (0.85 ml maximum capacity, less than 0.7 ml storage capacity, 0.4 ml elution capacity); 2304 in racks of 96; includes cap strips | 19588    |
| Collection Microtubes (racked)  | Nonsterile polypropylene tubes (1.2 ml), 960 in racks of 96   | 19560    |
| Collection Microtube Caps       | Nonsterile polypropylene caps for collection microtubes (1.2 ml) and round-well blocks, 960 in strips of 8  | 19566    |

### Related products for RNA purification from tissues

#### **RNeasy 96 Universal Tissue 8000 Kit — for automated purification of total RNA from any type of animal tissue using the BioRobot® Gene Expression — Real-Time RT-PCR workstation**

|  |   |         |
|--|---|---------|
| RNeasy 96 Universal Tissue 8000 Kit (12) | For 12 x 96 total RNA preps on the BioRobot Gene Expression — Real-Time RT-PCR workstation (based on the BioRobot 8000 platform):<br>12 RNeasy 96 Plates, Collection Microtubes (racked), Elution Microtubes CL (0.85 ml), Caps, Square-Well Blocks, AirPore Tape Sheets, RNase-Free Reagents and Buffers | Inquire |
|--|---|---------|

#### **MagAttract® RNA Tissue Mini M48 Kit — for automated purification of total RNA from clinical tissue samples using the BioRobot M48 workstation**

|  |  |        |
|--|--|--------|
| MagAttract RNA Tissue Mini M48 Kit (192) | For 192 RNA preps: MagAttract Suspension E, Buffers, 4 x RNase-Free DNase Sets, RNase-Free Water | 959336 |
|--|--|--------|

## Ordering Information

| Product  | Contents   | Cat. no. |
|--|--|----------|
| <b>EZ1 RNA Tissue Mini Kit — for automated purification of high-quality total RNA from tissue samples up to 10 mg using the BioRobot EZ1 workstation</b> |  |          |
| EZ1 RNA Tissue Mini Kit (48)   | For 48 RNA preps: 48 Reagent Cartridges (RNA Tissue), 100 Disposable Tip Holders, 100 Disposable Filter-Tips, 50 Sample Tubes (2 ml), 50 Elution Tubes (1.5 ml), RNase-Free DNase I, Buffers | 959134   |
| <b>EZ1 RNA Card — for easy setup of RNA purification protocols using the BioRobot EZ1 workstation and EZ1 RNA Kits</b>                                   |  |          |
| EZ1 RNA Card   | Pre-programmed card for EZ1 RNA purification protocols   | 9015590  |
| <b>RNeasy Protect Kits — for RNA/<i>later</i> stabilization and RNeasy purification of total RNA from animal tissues</b>                                 |  |          |
| RNeasy Protect Mini Kit (50)*  | RNA/ <i>later</i> RNA Stabilization Reagent (50 ml), 50 RNeasy Mini Spin Columns, Collection Tubes (1.5 ml and 2 ml), RNase-Free Reagents and Buffers  | 74124    |
| RNeasy Protect Midi Kit (10)*  | RNA/ <i>later</i> RNA Stabilization Reagent (20 ml), 10 RNeasy Midi Spin Columns, Collection Tubes (15 ml), RNase-Free Reagents and Buffers  | 75152    |
| RNeasy Protect Maxi Kit (12)   | RNA/ <i>later</i> RNA Stabilization Reagent (100 ml), 12 RNeasy Maxi Spin Columns, Collection Tubes (50 ml), RNase-Free Reagents and Buffers   | 75182    |

\* Larger kit sizes available; please inquire.

## Ordering Information

| Product   | Contents  | Cat. no. |
|---|---|----------|
| <b>RNeasy Lipid Tissue Kits — for purification of total RNA from fatty tissues</b>  |   |          |
| RNeasy Lipid Tissue Mini Kit (50)   | 50 RNeasy Mini Spin Columns, Collection Tubes (1.5 ml and 2 ml), QIAzol Lysis Reagent, RNase-Free Reagents and Buffers                | 74804    |
| RNeasy Lipid Tissue Midi Kit (10)   | 10 RNeasy Midi Spin Columns, Collection Tubes (15 ml), QIAzol Lysis Reagent, RNase-Free Reagents and Buffers                          | 75842    |
| <b>RNeasy Fibrous Tissue Kits — for purification of total RNA from fiber-rich tissues</b>                                   |   |          |
| RNeasy Fibrous Tissue Mini Kit (50)   | 50 RNeasy Mini Spin Columns, Collection Tubes (1.5 ml and 2 ml), Proteinase K, RNase-Free DNase I, RNase-Free Reagents and Buffers    | 74704    |
| RNeasy Fibrous Tissue Midi Kit (10)   | 10 RNeasy Midi Spin Columns, Collection Tubes (15 ml), Proteinase K, RNase-Free DNase I, RNase-Free Reagents and Buffers              | 75742    |
| <b>RNeasy Micro Kit — for purification of concentrated total RNA from small amounts of tissue or small numbers of cells</b> |   |          |
| RNeasy Micro Kit (50)   | 50 RNeasy MinElute Spin Columns, Collection Tubes (1.5 ml and 2 ml), RNase-Free DNase I, Carrier RNA, RNase-Free Reagents and Buffers | 74004    |

## Ordering Information

| Product   | Contents  | Cat. no. |
|---|---|----------|
| <b>Related products for RNA purification</b>  |   |          |
| <b>RNeasy 96 Kits — for high-throughput manual or automated RNA minipreps from cells</b>            |   |          |
| RNeasy 96 Kit (4)*  | For 4 x 96 total RNA preps:<br>4 RNeasy 96 Plates, Elution Microtubes CL, Caps, RNase-Free Reagents and Buffers   | 74181    |
| RNeasy 96 Kit (12)*   | For 12 x 96 total RNA preps:<br>12 RNeasy 96 Plates, Elution Microtubes CL, Caps, RNase-Free Reagents and Buffers   | 74182    |
| RNeasy 96 BioRobot 8000 Kit (12)  | For 12 x 96 total RNA preps on the BioRobot Gene Expression — Real-Time RT-PCR workstation (based on the BioRobot 8000 platform): 12 RNeasy 96 Plates, Elution Microtubes CL, Caps, Square-Well Blocks, RNase-Free Reagents and Buffers | 967152   |
| RNeasy 96 BioRobot 9604 Kit (12)  | For 12 x 96 total RNA preps on the BioRobot 9604: 12 RNeasy 96 Plates, Elution Microtubes CL, Caps, Square-Well Blocks, RNase-Free Reagents and Buffers   | 967142   |
| <b>RNeasy Kits — for purification of total RNA from animal cells or tissues, yeast, or bacteria</b> |   |          |
| RNeasy Mini Kit (50) <sup>†</sup>   | 50 RNeasy Mini Spin Columns, Collection Tubes (1.5 ml and 2 ml), RNase-Free Reagents and Buffers  | 74104    |
| RNeasy Midi Kit (10) <sup>†</sup>   | 10 RNeasy Midi Spin Columns, Collection Tubes (15 ml), RNase-Free Reagents and Buffers  | 75142    |

\* Requires use of QIAvac 96 or the QIAGEN 96-Well-Plate Centrifugation system.

<sup>†</sup> Larger sizes available; please inquire.



## Ordering Information

| Product  | Contents  | Cat. no. |
|--|---|----------|
| RNeasy Maxi Kit (12)   | 12 RNeasy Maxi Spin Columns, Collection Tubes (50 ml), RNase-Free Reagents and Buffers  | 75162    |
| <b>RNeasy MinElute Cleanup Kit — for RNA cleanup and concentration with small elution volumes</b>  |   |          |
| RNeasy MinElute Cleanup Kit (50)   | 50 RNeasy MinElute Spin Columns, Collection Tubes (1.5 ml and 2 ml), RNase-Free Reagents and Buffers  | 74204    |
| <b>Workstations for automated nucleic acid purification</b>  |   |          |
| <b>BioRobot Gene Expression system — for walkaway RNA purification and RT-PCR setup from animal tissue or cell culture samples in 96-well format</b> |   |          |
| BioRobot Gene Expression, Real-Time RT-PCR*  | Robotic workstation and Real-Time RT-PCR Specialist Pack, which includes QIAsoft 4.1 Operating System, chemistries starter kit, QIAsoft protocols, installation, training, and 1 year warranty on parts and labor | 9000710  |
| <b>BioRobot M48 workstation — for flexible, fully automated nucleic acid purification from 6–48 clinical samples</b>                                 |   |          |
| BioRobot M48*  | Robotic workstation for automated purification of nucleic acids using MagAttract M48 kits; computer, installation, 1 year warranty on parts and labor   | 9000708  |

\* QIAGEN Robotic Systems are not available in all countries; please inquire.

## Ordering Information

| Product   | Contents   | Cat. no. |
|---|--|----------|
| <b>BioRobot EZ1 workstation — for easy, automated purification of nucleic acids from 1–6 clinical samples</b>             |  |          |
| BioRobot EZ1*   | Robotic workstation for automated purification of nucleic acids using EZ1 kits; installation, 1 year warranty on parts and labor   | 9000705  |
| <b>BioRobot 9604 workstation — for automated nucleic acid purification from up to 96 clinical or cell-culture samples</b> |  |          |
| BioRobot 9604*  | Robotic workstation, computer-controlled vacuum pump, computer, QIAsoft 3.0 PLUS Operating System Basic Edition, installation and training, 1 year warranty on parts and labor                         | 900300   |
| <b>Products for downstream applications</b>   |  |          |
| <b>QuantiTect RT-PCR Kits — for quantitative, real-time one-step RT-PCR<sup>†</sup></b>                                   |  |          |
| QuantiTect SYBR® Green RT-PCR Kit (200) <sup>‡</sup>  | For 200 x 50 µl reactions:<br>3 x 1.7 ml QuantiTect SYBR Green RT-PCR Master Mix (providing a final concentration of 2.5 mM MgCl <sub>2</sub> ), 100 µl QuantiTect RT Mix, 2 x 2.0 ml RNase-Free Water | 204243   |
| QuantiTect Probe RT-PCR Kit (200) <sup>‡</sup>  | For 200 x 50 µl reactions:<br>3 x 1.7 ml QuantiTect Probe RT-PCR Master Mix (providing a final concentration of 4 mM MgCl <sub>2</sub> ), 100 µl QuantiTect RT Mix, 2 x 2.0 ml RNase-Free Water        | 204443   |

\* QIAGEN Robotic Systems are not available in all countries; please inquire.

<sup>†</sup> For more information about quantitative, real-time RT-PCR, request our application guide *Critical Factors for Successful Real-Time RT-PCR*.

<sup>‡</sup> Larger sizes available; please inquire.

# Ordering Information

| Product  | Contents  | Cat. no. |
|--|---|----------|
| <b>QuantiTect Gene Expression Assays — for gene expression analysis using functionally validated, ready-to-use, real-time RT-PCR assays*</b> |   |          |
| QuantiTect Gene Expression Assays (100)  | For 100 x 50 µl reactions (for use in a 96-well plate or single tubes) or 250 x 20 µl reactions (for use in a 384-well plate or single capillaries): 0.5 ml 10x QuantiTect Assay Mix (dyes available: FAM)  | Varies   |
| <b>QuantiTect Custom Assays — for gene expression analysis using custom-designed, quantitative, real-time RT-PCR assays*</b>                 |   |          |
| QuantiTect Custom Assay (500) <sup>†</sup>   | For 500 x 50 µl reactions (for use in a 96-well plate or single tubes) or 1250 x 20 µl reactions (for use in a 384-well plate or single capillaries): 1.25 ml 20x Primer Mix, 1.25 ml 20x QuantiProbe™ (dyes available: FAM, Yakima Yellow™, TET) | 241000   |
| <b>QIAGEN OneStep RT-PCR Kit — for easy and sensitive one-step RT-PCR</b>  |   |          |
| QIAGEN OneStep RT-PCR Kit (25) <sup>†</sup>  | For 25 reactions: QIAGEN OneStep RT-PCR Enzyme Mix, 5x QIAGEN OneStep RT-PCR Buffer (containing 12.5 mM MgCl <sub>2</sub> ), dNTP Mix (containing 10 mM each dNTP), 5x Q-Solution, RNase-Free Water   | 210210   |

\* For more information about quantitative, real-time RT-PCR, request our application guide *Critical Factors for Successful Real-Time RT-PCR*.

<sup>†</sup> Larger sizes available; please inquire.

QuantiTect Gene Expression Assays and QuantiTect Custom Assays or portions hereof are subject to proprietary rights of Epoch Biosciences, Inc. and are made and sold under license from Epoch under the patents and patent applications as may be designated by Epoch from time to time set forth, including one or more of the following: U.S. Patent Nos. 5,801,155, 6,084,102, 6,312,894, 6,426,408, and 6,127,121, and applications currently pending. Purchase of this product carries with it a limited, non-transferable, non-exclusive (without the right to resell, repackage, or sublicense) license under U.S. Patent Nos. 6,030,787; 5,723,591; and 5,876,930, and corresponding foreign patents.

Powered by innovation from Epoch Manufactured for QIAGEN by Epoch Biosciences

## Ordering Information

| Product   | Contents   | Cat. no. |
|---|--|----------|
| <b>Omniscript® RT Kit — for standard reverse transcription with any amount of RNA from 50 ng to 2 µg per reaction</b>               |  |          |
| Omniscript RT Kit (10)*   | For 10 reverse-transcription reactions: 40 units Omniscript Reverse Transcriptase, 10x Buffer RT, dNTP Mix (containing 5 mM each dNTP), RNase-Free Water   | 205110   |
| <b>Sensiscript® RT Kit — for reverse transcription using small amounts of RNA (i.e., less than 50 ng RNA including carrier RNA)</b> |  |          |
| Sensiscript RT Kit (50)*  | For 50 reverse-transcription reactions: Sensiscript Reverse Transcriptase, 10x Buffer RT, dNTP Mix (containing 5 mM each dNTP), RNase-Free Water   | 205211   |
| <b>HotStarTaq® DNA Polymerase — for robust amplification in all applications</b>  |  |          |
| HotStarTaq DNA Polymerase (250 U)*  | 250 units HotStarTaq DNA Polymerase, 10x PCR Buffer (containing 15 mM MgCl <sub>2</sub> ), 5x Q-Solution, 25 mM MgCl <sub>2</sub>  | 203203   |
| HotStarTaq Master Mix Kit (250 U)*  | 3 x 0.85 ml HotStarTaq Master Mix, containing 250 units HotStarTaq DNA Polymerase total and providing a final concentration of 1.5 mM MgCl <sub>2</sub> and 200 µM each dNTP; 2 x 1.7 ml distilled water | 203443   |
| <b>Taq DNA Polymerase — for standard and specialized PCR applications</b>   |  |          |
| Taq DNA Polymerase (250 U)*   | 250 units Taq DNA Polymerase, 10x PCR Buffer (containing 15 mM MgCl <sub>2</sub> ), 5x Q-Solution, 25 mM MgCl <sub>2</sub>   | 201203   |

\* Larger kit sizes available; please inquire.

## Ordering Information

| Product  | Contents  | Cat. no. |
|--|---|----------|
| <i>Taq</i> PCR Core Kit (250 U)*   | 250 units <i>Taq</i> DNA Polymerase, 10x PCR Buffer (containing 15 mM MgCl <sub>2</sub> ), 5x Q-Solution, 25 mM MgCl <sub>2</sub> , dNTP Mix (containing 10 mM each dNTP)                                   | 201223   |
| <i>Taq</i> PCR Master Mix Kit (250 U)*   | 3 x 1.7 ml <i>Taq</i> PCR Master Mix, containing 250 units <i>Taq</i> DNA Polymerase total and providing a final concentration of 1.5 mM MgCl <sub>2</sub> and 200 μM each dNTP; 3 x 1.7 ml distilled water | 201443   |
| <b>Custom DNA Oligos and Longmers — for custom synthesis of DNA oligos, including longmers and modified oligos</b> |   |          |
| Oligonucleotide Synthesis Service  | Custom-made oligonucleotides and a wide range of modified oligos, including Molecular Beacons, dual-labeled probes, and many more   | Inquire  |

\* Larger kit sizes available; please inquire.

## Notes

# QIAGEN Companies

Please see the back cover for contact information for your local QIAGEN office.

## QIAGEN Distributors

### Argentina

Tecnolab S.A.  
Tel: (011) 4555 0010  
Fax: (011) 4553 3331  
E-mail: info@tecnolab.com.ar  
Web site: www.tecnolab.com.ar

### Austria

VWR International GmbH  
Tel: (01) 576 00 0  
Fax: (01) 576 00 600  
E-mail: info@at.vwr.com  
Web site: www.vwr.com

### Belgium/Luxembourg

Westburg b.v.  
Tel: 0800-1-9815  
Fax: (31) 33-4951222  
E-mail: info@westburg.nl  
Web site: www.westburg.nl

### Brazil

Uniscience do Brasil  
Tel: 011 3622 2320  
Fax: 011 3622 2323  
E-mail: info@uniscience.com  
Web site: www.uniscience.com

### China

Gene Company Limited  
Tel: (852)2896-6283  
Fax: (852)2515-9371  
E-mail: info@genehk.com  
Hong Kong: info@genehk.com  
Beijing: info\_bj@genecompany.com  
Shanghai: info\_sh@genecompany.com  
Chengdu: gene@public.cd.sc.cn  
Guangzhou: info\_gz@genecompany.com

### Croatia

INEL Medicinska Tehnika d.o.o.  
Tel: (01) 2984-898  
Fax: (01) 6520-966  
E-mail: inel-medicinska-tehnika@zg.htnet.hr

### Cyprus

Scientronics Ltd  
Tel: 02-357 22 765416  
Fax: 02-357 22 764614  
E-mail: a.sarpetsas@biotronics.com.cy

### Czech Republic

BIO-CONSULT spol. s.r.o.  
Tel/Fax: (420) 2 417 29 792  
E-mail: info@bioconsult.cz  
Web site: www.bioconsult.cz

### Denmark

VWR International A/S  
Tel: 43 86 87 88  
Fax: 43 86 87 90  
E-mail: info@dk.vwr.com  
Web site: www.vwr.com

### Egypt

Clinilab  
Tel: 52 57 212  
Fax: 52 57 210  
E-mail: Clinilab@link.net

### Finland

VWR International Oy  
Tel: (09) 804 551  
Fax: (09) 8045 5200  
E-mail: info@fi.vwr.com  
Web site: www.vwr.com

### Greece

BioAnalytica S.A.  
Tel: (210)-640 03 18  
Fax: (210)-646 27 48  
E-mail: bioanalyt@hol.gr  
Web site: www.bioanalytica.gr

### Hungary

Kasztel-Med Co. Ltd.  
Tel: (01) 385 3887  
Fax: (01) 381 0695  
E-mail: info@kasztel.hu  
Web site: www.kasztel.hu

### India

Genetix  
Tel: (011)-2542 1714  
or (011)-2515 9346  
Fax: (011)-2546 7637  
E-mail: genetix@nda.vsnl.net.in

### Israel

Westburg (Israel) Ltd.  
Tel: 08-6900655  
or 1-800 20 22 20 (toll free)  
Fax: 08-6900650  
E-mail: info@westburg.co.il  
Web site: www.westburg.co.il

### Korea

LRS Laboratories, Inc.  
Tel: (02) 924-86 97  
Fax: (02) 924-86 96  
E-mail: webmaster@lrslab.co.kr  
Web site: www.lrslab.co.kr

### Malaysia

RESEARCH BIOLABS SDN. BHD.  
Tel: (603)-8070 3101  
Fax: (603)-8070 5101  
E-mail: biolabs@tm.net.my  
Web site: www.researchbiolabs.com

### Mexico

Quimica Valaner S.A. de C.V.  
Tel: (55) 55 25 57 25  
Fax: (55) 55 25 56 25  
E-mail: ventas@valaner.com  
Web site: www.valaner.com

### The Netherlands

Westburg b.v.  
Tel: (033)-4950094  
Fax: (033)-4951222  
E-mail: info@westburg.nl  
Web site: www.westburg.nl

### New Zealand

Biolab Ltd  
Tel: (09) 980 6700  
or 0800 933 966  
Fax: (09) 980 6788  
E-mail: biosciences@nzl.biologbgroup.com  
Web site: www.biologbgroup.com/nzl

### Norway

VWR International AS  
Tel: 02 29 0  
Fax: 22 90 00 40  
E-mail: info@no.vwr.com  
Web site: www.vwr.com

### Poland

Syngen Biotech Sp.z.o.o.  
Tel: (071) 351 41 06  
or 0601 70 60 07  
Fax: (071) 351 04 88  
E-mail: info@syngen.pl  
Web site: www.syngen.pl

### Portugal

IZASA PORTUGAL, LDA  
Tel: (21) 424 7312  
Fax: (21) 417 2674  
E-mail: consultasbiotec@izasa.es

### Singapore

Research Biolabs Pte Ltd  
Tel: 67775366  
Fax: 67785177  
E-mail: sales@researchbiolabs.com  
Web site: www.researchbiolabs.com

### Slovak Republic

BIO-CONSULT Slovakia spol. s.r.o.  
Tel/Fax: (02) 5022 1336  
E-mail: bio-cons@edicon.sk  
Web site: www.bioconsult.cz

### Slovenia

MEDILINE d.o.o.  
Tel: (01) 830-80-40  
Fax: (01) 830-80-70  
or (01) 830-80-63  
E-mail: mediline@sicl.net

### South Africa

Southern Cross Biotechnology  
(Phy) Ltd  
Tel: (021) 671 5166  
Fax: (021) 671 7734  
E-mail: info@scb.co.za

### Spain

IZASA, S.A.  
Tel: (93) 902.20.30.90  
Fax: (93) 902.22.33.66  
E-mail: consultasbiotec@izasa.es

### Sweden

VWR International AB  
Tel: (08) 621 34 00  
Fax: (08) 760 45 20  
E-mail: info@se.vwr.com  
Web site: www.vwr.com

### Taiwan

TAIGEN Bioscience Corporation  
Tel: (02) 2880 2913  
Fax: (02) 2880 2916  
E-mail: taigen@ms10.hinet.net

### Thailand

Theera Trading Co. Ltd.  
Tel: (02) 412-5672  
Fax: (02) 412-3244  
E-mail: theera@samart.co.th

### Turkey

Medek Medikal Ürünler  
ve Sağlık Hizmetleri A. S.  
Tel: (216) 302 15 80  
Fax: (216) 302 15 88  
E-mail: makalp@med-ek.com

### All other countries

QIAGEN GmbH, Germany

**Australia** = **QIAGEN Pty Ltd** = ABN 75 072 382 944 = PO Box 25 = Clifton Hill = Victoria 3068  
Orders 03-9489-3666 = Fax 03-9489-3888 = Technical 1-800-243-066

**Canada** = **QIAGEN Inc.** = 2800 Argentia Road = Unit 7 = Mississauga = Ontario = L5N 8L2  
Orders 800-572-9613 = Fax 800-713-5951 = Technical 800-DNA-PREP (800-362-7737)

**France** = **QIAGEN S.A.** = 3 avenue du Canada = LP 809 = 91974 COURTABOEUF CEDEX  
Orders 01-60-920-920 = Fax 01-60-920-925 = Technical 01-60-920-930

**Germany** = **QIAGEN GmbH** = QIAGEN Strasse 1 = 40724 Hilden  
Orders 02103-29-12000 = Fax 02103-29-22000 = Technical 02103-29-12400

**Italy** = **QIAGEN S.p.A.** = Via Grosio, 10/10 = 20151 Milano  
Orders 02-33430411 = Fax 02-33430426 = Technical 02-33430414

**Japan** = **QIAGEN K.K.** = Forefront Tower II = 13-1, Kachidoki 3 Chome = Chuo-ku, Tokyo 104-0054  
Telephone 03-5547-0811 = Fax 03-5547-0818 = Technical 03-5547-0811

**Switzerland** = **QIAGEN AG** = Auf dem Wolf 39 = 4052 Basel  
Orders 061-319-30-30 = Fax 061-319-30-33 = Technical 061-319-30-31

**UK and Ireland** = **QIAGEN Ltd.** = QIAGEN House = Fleming Way = Crawley = West Sussex, RH10 9NQ  
Orders 01293-422-911 = Fax 01293-422-922 = Technical 01293-422-999

**USA** = **QIAGEN Inc.** = 27220 Turnberry Lane = Valencia = CA 91355  
Orders 800-426-8157 = Fax 800-718-2056 = Technical 800-DNA-PREP (800-362-7737)

